



LABORATORY V. 5.2

ISBT USER GUIDE

VistA BLOOD BANK SOFTWARE

March 2001

Department of Veterans Affairs
VISTA System Design and Development

TABLE OF CONTENTS

INTRODUCTION.....	1
Scope of This User Guide	1
Definitions	3
References	5
DESCRIPTION OF SOFTWARE CHANGES.....	6
Specific File and Field Changes	7
ISBT 128 BARCODE CHARACTERISTICS FOR U.S. IMPLEMENTATION.....	9
Codabar Limitations and the Code 128 Character Set	9
Component Elements of ISBT 128 Barcodes.....	9
Structure of ISBT 128 Blood Product Description	11
IMPLEMENTING CHANGES INTRODUCED BY LR*5.2*267.....	13
SETTING UP A NEW ENTRY IN THE BLOOD PRODUCT FILE (#66):.....	15
CHANGES IN SPECIFIC OPTIONS.....	23
BP Edit Blood Product File [LRBLSEB].....	23
LR Log-in Regular (Invoices) [LRBLILR]	25
DN Disposition – Not Transfused [LRBLIDN]	27
PD Pediatric Unit Preparation [LRBLPED].....	30
ADDITIONAL OPTIONS MODIFIED.....	33
Options Modified to Accept Barcode Scanner Input for an ISBT 128 Unit ID Barcode	33
Options Modified to Accept Manual Data Input of a 13 Character ISBT 128 Unit ID.....	33
Options and Reports Modified to Print and/or Display the Longer ISBT 128 Unit ID	34
APPENDIX A - SUPPLIER MULTIPLE ENTRIES FOR ARC.....	35
APPENDIX B - US ISBT 128 PRODUCT CODES	36
INDEX.....	137

Introduction

Laboratory patch LR*5.2*267 provides partial implementation of the ISBT 128 barcode capability, and a fix for a problem with the option Pediatric unit preparation [LRBLPED]. A partial implementation is provided at this time in order to remain current with best practice policies, the new international standard, and to allow sites to process ISBT128-labeled units in a normal manner without a manual workaround. A full implementation shall be provided in a future product release.

The International Society of Blood Transfusion (ISBT) established a working group on automation and data processing to establish a replacement for the currently used ABC Codabar, which has reached a useful limit in a world of increasing information complexity. Code 128 was chosen because it codes more data into a smaller space, easily handles alphanumeric data, provides for internal scanning error checks, and supports concatenation (allows reading more than one barcode symbol with a single scan). The ISBT work group was joined by the American Association of Blood Banks (AABB), the American Red Cross (ARC), the Department of Defense (DoD), and the Health Industry Manufacturers Association. As a result, ISBT 128 was adopted as an international standard.

A deficiency in the option Pediatric unit preparation [LRBLPED] is also being corrected. Previously, this option allowed users to create new unit records containing blood product from existing units. However, in the creation of the records, new units were not assigned a division to which they should belong. As a result, units created through this option were unusable in the rest of the system. This option is fixed so that each unit created will be assigned the division of the creating user.

Scope of This User Guide

This ISBT User Guide provides instructions and a description of changes for those options that are affected by patch LR*5.2*267. This guide is not designed to be fully inclusive of all functionality associated with any particular option described. For additional setup and operating information, refer to the original Blood Bank Software User Manual V. 5.2, distributed in October 1994.

This user guide can be used as an example to follow when scanning and performing manual entries of ISBT 128 labels. Although the software has been altered to enable the reading of ISBT 128 labels as well as Codabar labels, the methods of using the software have not changed significantly. The most significant change is to accommodate the 13-character Unit ID present with ISBT 128-labeled units, while still maintaining a readable display of information presented to the user. Additional changes of significance affect the functionality associated with creating Divided units using the option Disposition – not transfused [LRBLIDN] and Pediatric unit preparation [LRBLPED].

Note: It should be noted that the behavior of these two options is different depending upon whether the original (parent) unit is labeled as ISBT 128 or Codabar.

Associated Documents Released with Patch LR*5.2*267

The release of patch LR*5.2*267 is accompanied by the release of the following documents in addition to this ISBT 128 User Guide:

- Appendix C to the ISBT User Guide-Test Plan. This appendix is released as a separate document. This document contains:
 - Test scripts reflecting normal conditions of options affected by changes in LR*5.2*267 using both ISBT 128 and Codabar examples. These test scripts can also be used as worksheets to document validation performed
 - Sample ISBT 128 labels that can be used to assist sites with validation of ISBT 128 functionality
 - Instructions for BLOOD PRODUCT File (#66) definitions for both the CODABAR and ISBT 128 product types used to create the test scripts
- Appendix E to the Blood Bank User Manual v 5.2. This is a revised version of Appendix E and is intended to replace the previously released Appendix E dated July 1996. This manual contains:
 - General guidance to be used for the validation of blood bank software
 - Details of control functions for all options in the VistA Blood Bank Software v 5.2
 - Sample forms for use in managing change control
 - Sample test case tracking worksheets
 - A Frequently Asked Questions (FAQ) section containing questions and answers to commonly asked questions concerning the VistA Blood Bank Software v 5.2.

Definitions

AABB

American Association of Blood Banks. This is a regulatory agency that focuses on quality practices within a blood bank and transfusion service.

ARC

American Red Cross.

CCB

Change Control Board. This is a governing body that reviews and approves functionality included in the blood bank software.

Code 128

Code 128 is a very high-density alphanumeric barcode that allows for more information to be coded into a small space and includes an internal check digit to prevent barcode misreads.

Codabar

The Codabar barcode font is used for various numeric barcoding applications including libraries, blood banks and parcels. Codabar was designed for character self-checking eliminating the requirement for checksum characters. However, checksum characters in the Codabar barcode are optional and they do maximize data integrity.

DoD

Department of Defense.

FDA

Food and Drug Administration.

ICCBBA

International Council for Commonality in Blood Banking Automation. This group was tasked with developing the implementation of the ISBT 128 blood product labeling standard.

ISBT

International Society of Blood Transfusion.

ISBT 128

ISBT 128 is an international standard for the uniform labeling of blood products. It has many features, some of which are not being implemented at this time. The major features are:

- Highly structured Product Description (i.e. product naming convention)
- Highly structured Donation Identification Number (collection information embedded within Unit ID barcode)
- Strict standards as to the layout of a blood product label
- Expanded information embedded within the ABO/Rh label
- Standard format for the expiration date label
- Supports concatenation—that is the reading of two barcodes using one scan
- Utilizes Code 128 symbology for barcodes as opposed to Codabar

SRS

Software Requirements Specification. This is a document that details the functionality included in a software application.

VBECs

VistA Blood Establishment Computer Software. The name of the proposed replacement for the current VistA Blood Bank Software v 5.2.


VISTA

Veterans Health Information Systems and Technology Architecture.

References

United States Industry Consensus Standard for the Uniform Labeling of Blood and Blood components using ISBT 128, version 1.2.0 *Published by the International Council for Commonality in Blood Banking Automation, Inc., November 1999.*

SAMPLE ISBT 128 BARCODE LABEL

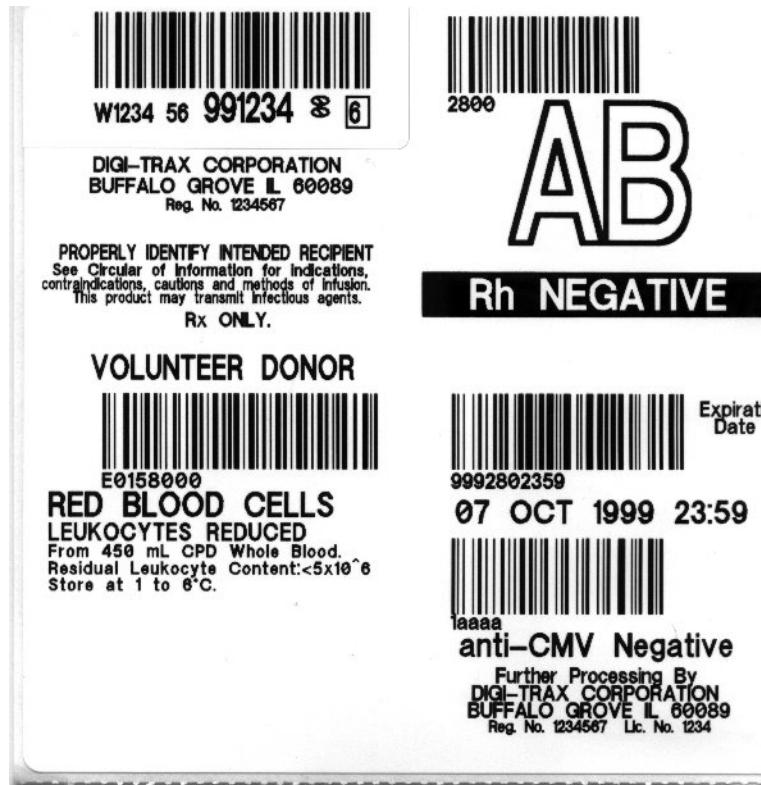

Description of Software Changes

- The field length for the BLOOD INVENTORY File (#65) field UNIT ID (#65,.01) and the BLOOD PRODUCT File (#66) field PRODUCT CODE (#66,.05) have been modified to accept the longer Unit ID and Product Codes that are ISBT 128 uses.
- A new field in the BLOOD PRODUCT File (#66) to establish a relationship between ISBT 128 product codes and Codabar product codes has been added. Logic has been added to the input transform of the BLOOD PRODUCT File (#66) field MODIFY TO (#66.03,.01) to restrict modifications of ISBT 128 units to other ISBT 128 blood component types. The logic also restricts the modification of Codabar units to other Codabar unit types.
- The ability to read and interpret the various ISBT 128 barcodes has been provided, but sites will be required to maintain ISBT 128 component types within the current BLOOD PRODUCT File (#66) structure. Unit ID, ABO/Rh., Product Code, and Expiration Date barcode labels are now supported. None of the additional information that is embedded within the ISBT 128 barcode labels can be extracted.
- Sites creating pooled products will need to maintain off-line a system to name their pools using the ISBT 128 standards but VistA will be able to accept those pool names. This is consistent with the current Codabar functionality.
- VistA Blood Bank Reports and displays will be adjusted to accommodate the longer field lengths.
- On-demand printing of full-face blood bag labels is not supported. Sites will need to purchase pre-printed labels for products modified in the facility. (See International Council for Commonality in Blood Banking Automation(ICCBBA) GUIDANCE FOR INDUSTRY—United States Industry Consensus Standard for the Uniform Labeling of Blood and Blood Components using ISBT 128, Sec. 4.5).
- No enhancements have been made to the current VistA Donor package to bring it into ISBT 128 compliance since there will be no Donor support in the VistA Blood Establishment Computer Software(VBECs).
- The current Codabar parser has been modified to recognize an ISBT 128 unit and an additional parser routine has been written to interpret these barcodes.
- Current user and technical reference documentation has been issued to reflect the new partial ISBT 128 labeling standard.

Specific File and Field Changes

Because of time constraints and FDA regulations regarding changes made to a cleared medical device, the current application can only partially implement the ISBT 128 system. However, these changes will enable sites to process blood components labeled using ISBT 128 with the same level of confidence that the current Codabar system provides. The additional features provided by the ISBT 128 system will be implemented at a future date. Minimal changes have been made to the following files/fields to accommodate ISBT 128:

BLOOD PRODUCT File (#66) changes:

New fields:

IS ISBT128 (#66,.29): Required field is a set of codes—Yes or No. This field indicates whether the product type belongs to ISBT 128 or to Codabar. All product types fall into one of two categories: Codabar or ISBT 128. This field identifies the symbology to which each product type belongs. During installation of this patch, all current entries of the BLOOD PRODUCT File (#66) will be set to NO.

EQUIVALENT PRODUCT (#66,9): This field points to the blood product (of the opposite symbology) that most closely matches or is equivalent to the specified blood product. It screens on the IS ISBT field and allows only blood products of opposite symbologies to be stored as equivalent products. For any ISBT 128 products, only products with IS ISBT = NO (Codabar products) can be selected. The same is true for Codabar units; only blood products with IS ISBT = YES (ISBT 128 products) can be selected. Although not required, assigning a value to this field when creating ISBT 128 product types will assist in the data conversion that will be done when migrating to a new Blood Bank application.

Changes made to existing fields:

PRODUCT CODE (#66,.05): Maximum field length increased to accommodate the 8 character ISBT 128 product code.

MODIFY TO (#66.03,.01): Additional screen entered to restrict choices to BLOOD PRODUCT File (#66) entries of the same symbology, based on the entry of the IS ISBT128 field of the parent and possible child product types.

PEDIATRIC PRODUCT (#66,.22): Additional screen entered to restrict choices to BLOOD PRODUCT File (#66) entries of the same symbology, based on the entry of the IS ISBT128 field of the parent and possible child product types.

BLOOD INVENTORY File (#65) changes:

Changes made to existing fields:

UNIT ID (#65,.01): Maximum field length increased to accommodate the 13 character ISBT 128 Donation Identification Number.

PEDIATRIC ALIQUOT MADE (#65.16,.01): Maximum field length increased to accommodate the 13 character ISBT 128 Donation Identification Number.

UNIT ID (#65.091,.02): This is the UNIT ID's of child units created from a parent unit through modification. Maximum field length increased to accommodate the 13-character ISBT 128 Donation Identification Number.

LAB DATA File (#63) changes:

Changes made to existing field:

COMPONENT ID (#63.017,.03): This is where the UNIT ID of a transfused unit is stored for a patient. Maximum field length increased to accommodate the 13-character ISBT 128 Donation Identification Number.

ISBT 128 Barcode Characteristics for U.S. Implementation

The following topics discuss the reasons for changing to ISBT 128 barcodes, and specific characteristics of ISBT 128 labels and coding formats.

Codabar Limitations and the Code 128 Character Set

Codabar Product Codes were originally designed as five-digit structured codes. Characters one through three described the product's proper name, the fourth character described the anticoagulant, and the fifth character described any specifics as to the content. As product types became more numerous, the structure of this code could no longer accommodate the numbers of product types, and currently there is no longer any conformity to this standard. It became obvious that a new standard would need to be devised.

There is a lack of consistency between various blood collection agencies as to how they implemented the Codabar unit ID barcode label. Although the Codabar unit ID reads only as a numeric, the visual interpretation must be calculated based on the labeling preferences of the specific blood collection facility. For example, a Codabar unit ID that scans as 0316165 can be visually interpreted as either G16165 or 0316165, and the unit of blood may also have appended to it a two-digit, eye-readable prefix in the range of 01-99. This demonstrates that the Codabar Unit ID as scanned can have multiple visual interpretations.

There is also a lack of consistency between the various blood collection agencies regarding the implementation of the Codabar expiration date label.

ISBT 128 uses Code 128 barcode symbology, which recognizes a larger character set, allowing more information to be included in the barcode. The new standard was created to standardize all aspects of blood components labeling, thereby creating a system that is consistent, expandable, predictable, and that provides for the unique identification of any blood component for a period of 100 years.

Component Elements of ISBT 128 Barcodes

Donation Identification Number (Unit ID)—Data structure *opppp yy nnnnnn*

- Located at the uppermost left of the blood component label.
- The barcode consists of 13 data characters, a data identifier and flag characters. The data identifier is embedded within the barcode and is used to identify the type of barcode being scanned.
 - A. *opppp*—designates the country and collection facility.
 - B. *yy*—designates the year in which the donation or collection was made.
 - C. *nnnnnnn*—is the serial number associated with the donation or collection.
- Provides for the unique identification of any donation or collection world-wide for a one hundred year period.
- An additional check digit calculated on the 13 data characters is printed in a box to the right of the Donation Identification Number. In a future application this will be used to validate the accuracy of manual data entry.

- A hidden data identifier is embedded within the barcode to identify the barcode as a Donation Identification Number barcode.
- Flag characters (displayed either rotated 90 degrees or in icon format) are the last two characters of the Donation Identification Number data structure. They are not part of the Donation Identification Number. In the US application of ISBT 128, these will always default to 00. As recommended by the US Industry Consensus Standard for ISBT 128, the current application will ignore them from the scanned data input.
- Example of typical ISBT 128 Donation Identification Number: W123401123456

Product Code—Structure *E0000tds*:

- Located at the center-left of the blood component label.
- The barcode consists of 8 characters plus a hidden data identifier. The data identifier is embedded within the barcode and is used to identify the type of barcode being scanned. The structure of the 8 character code is as follows:
 - ***E0000***—5 characters used for the product description. This is a random number assigned to a specific product type by the ICCBBA. E was chosen as the first alpha character to be used since A, B, C and D were used by Codabar as start/stop characters.
 - ***t***—One character to designate the type of donation or collection/intended use.
 - ***ds***—provides information about the division of a product. Will be 00 unless the unit has been split from a parent unit.
 - Example of typical Product Code, using AS-1 Red Blood Cells as the example: E0291000

ABO/Rh Blood Groups—Structure *ggre*

- Located at the uppermost-right of the blood component label.
- The barcode consists of 4 characters plus a hidden data identifier. The data identifier is embedded within the barcode and is used to identify the type of barcode being scanned.
 - ***gg*** - designates the ABO and Rh group according to a table supplied by ICCBBA.
 - ***r*** - designates special testing but is not used in the US Implementation and will default to 0.
 - ***e*** - is reserved for future use and will default to 0.
- The ISBT 128 ABO/Rh group codes are expanded from the current Codabar codes, and in the US implementation, information about the type of donation/intended use is included in the ABO/Rh blood group barcode. The current application will only extract the ABO and Rh blood group information from this label.
- Example of a typical ISBT 128 ABO/Rh barcode using O Pos as the example:
5100

Expiration Date/time—Structure *cyyjjjhmm*

- Located in the center-right of the blood component label.
- The barcode consists of 10 data characters plus a hidden data identifier. The data identifier is embedded within the barcode and is used to identify the type of barcode being scanned.
- *c* - designates the century (e.g. 9 for 1999, 0 for 2000)
- *yy* -- designates the year
- *jjj* -- is the julian date (the number of the day in the year)
- *hh* -- specifies the hour (0-23)
- *mm* -- specifies the minutes (00-59)
- an example of a coded expiration date would be: 0011422359
- The structure of the displayed expiration date is: DD MMM YYY HR:MIN
- The US Implementation always will include the time in the data structure. When not a time dependent blood product, the time is encoded as 23:59. When this 23:59 time is used, it is not necessary that this time be displayed in the barcode text and a midnight time should be assumed.
- An example of a displayed expiration date would be 22 MAY 2001 23:59.

Special Testing -Structure *1aaaaa*

- Located in the bottom most right of the blood component label.
- Consists of 5 data characters plus a hidden data identifier. The data identifier is embedded within the barcode and is used to identify the type of barcode being scanned.
- In the US Implementation, only anti-CMV status will be encoded here.
- This barcode will be utilized in a future application and will not be interpreted by the current software.

NOTE: In ISBT 128, there is no FDA Registration facility barcode. The identification of the collection facility is embedded within the Donation Identification Number.

Structure of ISBT 128 Blood Product Description

Although there is no structure to the five-character ISBT 128 Product Code, the ISBT 128 Labeling Standard does provide a very structured format for the Blood Product Description. All blood component names follow the following format:

Blood Component|Core Condition|Other Attributes|Other Attributes

Any blood component can also have one or more modifiers in addition to a core condition and other attributes. Depending on the amount of further processing that is done on any particular blood component, this Blood Product Description may become very long. Due to the constraints of the current VA FileMan system, it will not be practical to attempt to use the ISBT 128 Blood Product Description as the NAME field in the BLOOD PRODUCT File (#66) when creating new entries for some of these ISBT 128 product types.

An example of the ISBT 128 Blood Product Description for an AS-1 Red Blood Cell component would look like this:

RED BLOOD CELLS|AS1/450mL/refr
The ISBT 128 Product code is E0291000

An example of the ISBT 128 Product Description for this same AS-1 Red Blood Cell component after processing into an irradiated and leuko-poor component would be:

RED BLOOD CELLS|AS1/450mL/refg|Irradiated|ResLeu:<5log6
The ISBT 128 Product Code is now E0307000

Definitions of Terms:

1. **BLOOD COMPONENT:** Consists of the component class (required) and any modifiers (optional)
 - A. **COMPONENT CLASS:** General description of the cellular and/or non-cellular product having a unique set of core conditions, e.g. Red Blood Cells, Whole Blood, Plasma, Platelets
 - B. **MODIFIER:** A description that relates to the core conditions of a blood component class that distinguishes it from other members of the same component class, e.g. Frozen, Frozen Rejuvenated, Washed.
2. **CORE CONDITIONS:** Consists of three parts, anticoagulant or additive if present, nominal volume of original collection and relevant storage temperature. These are delimited by the slash “/”, e.g. AS3/450 ml/refr
3. **OTHER ATTRIBUTES:** A blood product may be further defined by the inclusion of attribute variables from one or more attribute groups. Unless otherwise stated, the default state of a product is assumed, e.g. is intended for transfusion and was prepared in a closed system, not exposed to radiation, not leuko-reduced etc. Other Attributes are organized into the following groups:
 - A. Intended Use.
 - B. System Integrity.
 - C. Irradiation.
 - D. Residual Leukocyte Count.
 - E. Altered.
 - F. Final Content.
 - G. Additional information on preparation.
 - H. Apheresis.
 - I. Quarantine.
 - J. Pools - number of donors in a pool or approximate number of platelets in pool.
 - K. Method of treatment.

Implementing Changes Introduced By LR*5.2*267

PREPARATION FOR INSTALLATION OF LR*5.2*267

No advance site preparation is necessary prior to the installation of LR*5.2*267.

Prior to installation of the patch, it is recommended that blood bank users should read this user guide along with the Laboratory V. 5.2 ISBT User Guide – Appendix C - Test Plan. Installation and validation should first be undertaken in a mirrored test account if at all possible. Sample ISBT 128 labels are included in the Laboratory V. 5.2 ISBT User Guide – Appendix C - Test Plan for your convenience in creating sample ISBT 128 blood product types.

BARCODE SCANNER CONSIDERATIONS

Use of a barcode scanner in the blood bank is recommended in order to achieve the maximum benefits of the software and to improve accuracy and safety. Currently in the field the barcode scanners in use are only required to read and interpret Codabar symbology. In order to process blood components using the ISBT 128 standard, it is necessary that the blood bank have a scanner that can auto-discriminate between Codabar and Code 128 symbologies; that is, be able to read both types of symbologies without the need to alter the setup of the scanner for each symbology. The sample ISBT 128 labels that are included in the Laboratory V. 5.2 ISBT User Guide – Appendix C - Test Plan can be used to test the ability of your scanner to do this. Refer to the setup manual that came with your scanner or contact the manufacturer for additional guidance. Scanners should be configured to automatically execute a carriage return after each scan. The following scanners were used in the development and testing of patch LR*5.2*267:

- Symbol Technologies LS 2000MX
- Symbol Technologies LS 4000i

OVERVIEW OF FUNCTIONAL CHANGES:

Changes in the blood bank software function after installation of patch LR*5.2*267 are:

- The option Edit blood product file [LRBLSEB] prompts for the two new fields in the BLOOD PRODUCT File (#66). These new fields are the IS ISBT128 (#66,.29) and the EQUIVALENT PRODUCT (#66,9) fields.
- The option Edit blood product file [LRBLSEB] prompts for the ASSOCIATED DIVISION field (#66.1,.01) earlier in the definition of a new blood product. It is prompted for immediately after the IS ISBT128 field (#66,.29).

- Prior to installation of LR*5.2*267, for prompts designed to accept scanner input, the screen echoes what the scanner literally reads and then re-displays the interpretation of the reading. After installation of this patch, users may notice that the echo of the literal scanned input may display for a split second and be erased prior to the display of the interpretation. This is normal and intentional. Users will notice this split-second display-erase-redisplay for data input at these prompts for both barcode and manual data entry.
- Changes are made to the option Disposition –not transfused [LRBLIDN] when processing an ISBT 128 product type into divided units. The system is designed to know if the parent unit is labeled using Codabar or ISBT 128 based on the entry in the IS ISBT128 field (#66,.29) in the BLOOD PRODUCT File (#66). Prior to processing an ISBT 128 blood component into aliquots, sites are required to create unique entries in the BLOOD PRODUCT File (#66) for each possible number of aliquots created. For example, if a site splits a component into three aliquots, three separate entries must be created in the BLOOD PRODUCT File (#66) for the divided products. The processing of a Codabar unit into divided products remains unchanged.
- Changes are made to the option Pediatric unit preparation [LRBLPED]. The system is designed to know if the parent unit is labeled using Codabar or ISBT 128 based on the entry in the IS ISBT 128 field (#66,.29) in the BLOOD PRODUCT File (#66). Prior to processing an ISBT 128 blood component into aliquots, sites are required to create unique entries in the BLOOD PRODUCT File (#66) for each possible number of aliquots created. Theoretically, this could be up to 26 since the Pediatric unit preparation option allows up to 26 aliquots to be created from a single unit. The creation of pediatric aliquots from a Codabar component remains unchanged.
- The option Pediatric unit preparation [LRBLPED] now assigns the division of the user to each pediatric aliquot created.

Setting Up a New Entry in the Blood Product File (#66):

The following instructions are being provided to assist sites in creating new entries into the BLOOD PRODUCT File (#66) using the option Edit blood product file [LRBLSEB]. The instructions may also be useful to assist sites in better understanding how entries in specific fields in this file affect the characteristics of specific blood components.

Several changes will be noted in the Edit blood product file [LRBLSEB] option after installation of patch LR*5.2*267:

- A new required field has been added called IS ISBT 128 (#66,29). This is a YES/NO field . As part of the installation process of LR*5.2*267, a value of NO is assigned to all existing records in this file.
- A new field has been added called EQUIVALENT PRODUCT (#66,9). This field is a pointer to the BLOOD PRODUCT File (#66). It is screened to allow only BLOOD PRODUCT File entries with non-identical entries in the IS ISBT 128 field.
- The input template for this option now prompts for input of the ASSOCIATED DIVISION field (#66,10) immediately after the IS ISBT 128 field.

The most significant difference between setting up a blood component labeled using ISBT 128 as opposed to one labeled using Codabar is in the definition of fields in the SUPPLIER multiple. In Codabar, because of the possibility of an eye-readable prefix, and totally numeric vs. alpha characters and any combination of these components being processed at a site, separate entries in the SUPPLIER multiple were recommended for each component type defined. This ensured that scanning of the Unit ID field would be interpreted properly when used in conjunction with the proper SUPPLIER multiple entry. In ISBT 128, the Unit ID field format is consistent, therefore, multiple SUPPLIER entries for any specific ISBT labeled product are only necessary if the site has different sources of the same component and wishes to track separate costs.

NOTE: See Appendix A for the current listing of American Red Cross (ARC) collection facilities, prefixes, and FDA registration numbers.

BLOOD PRODUCT FILE #66

NAME Field # .01: This is the name of the specific product. Although the field allows 40 characters, the most relevant information should be contained within the first 30 characters. Because of the limitations of the current file structure and how FileMan is used for sorting file entries, it may not be practical to enter the official ISBT 128 Product Description as the BLOOD PRODUCT NAME. In this application, the PRODUCT CODE will be the key entry to define a specific blood product, whether it is Codabar or ISBT 128 labeled.

ABBREVIATION Field # .02: A shortened name for a blood product-- must be between 1-4 characters. Can be used to lookup an existing entry.

CAN BE MODIFIED Field # .03: This is a yes/no field. If the blood component type can be modified into another blood component type, then a YES should be entered here.

IDENTIFIER Field # .04:

This field is a set of codes. Valid choices are:

BB:COMPONENT/DERIVATIV (always choose **BB** when defining a new blood product)

AB:ANTISERUM (not currently used by application)

T:TEST PROVIDED (limited use, TYPING CHARGE entry only)

PRODUCT CODE Field # .05: This is the unique code assigned to a blood product. In Codabar, it is always a 5-number code. In ISBT 128, the product description is coded within the first five characters, the donation type is encoded within the 6th character and characters 7-8 are reserved to identify the split (aliquot) level. In this VistA application, we will not decode the 6th character, donation type, however it must be entered as provided by your blood supplier for the product to be scanned properly. If the product being defined is a divided or Pediatric product, a unique product code for each split (aliquot) level possible must be entered here in the format α0000tA0, α0000tB0, α0000tC0. In order to provide for uniqueness in the BLOOD INVENTORY File (#65), there must be a unique entry in the BLOOD PRODUCT File (#66) for each possible aliquot that can be prepared from a parent unit. The α0000t portion of the ISBT 128 product code must be the same as the parent unit, and each additional aliquot that can be prepared must follow the format A0, B0, C0, D0 in characters 7-8.

IS ISBT128 Field # .29: This is a new yes/no field. It is required and will be used in conjunction with the MODIFY TO field to restrict component modifications to blood components of like symbology. Answer YES if the blood component type is labeled using ISBT 128. Answer NO if the blood component type is labeled using Codabar.

Select **ASSOCIATED DIVISION Field # 10:** This is a required, multiple field and identifies the division(s) with which a specific blood component type can be associated.

ASSOCIATED DIVISION Field # 66.1,.01: A separate entry must be made for each valid division within a multi-divisional institution that can receive and process a specific blood component type.

DOD CODE Field # .055: This field is not currently used.

MODIFICATION CRITERIA Field # .06: This field controls the software behavior when using the option Disposition –not transfused [LRBLIDN] to modify a blood component into another, different blood component. An entry is made in this field when defining the ‘child’ product type, not the parent. For example, D should be entered here if the product being defined is a Divided Unit.

PATIENT/PRODUCT ABO Field # .07: Choices are MUST MATCH or MUST BE COMPATIBLE. The entry here controls the checks that are made when selecting specific blood components for a patient. MUST MATCH will only allow units of the same ABO as a patient, MUST BE COMPATIBLE will allow selection of units based on currently acceptable ABO substitutions, based on the entry in the PATIENT/PRODUCT REQUIREMENT field for this product.

PATIENT/PRODUCT RH Field # .08: Choices are MUST MATCH or MUST BE COMPATIBLE. The response here controls the checks that are made when selecting specific blood components for a patient. MUST MATCH will only allow units of the same Rh as a patient, MUST BE COMPATIBLE will allow selection of units based on currently acceptable Rh substitutions, based on the entry in the PATIENT/PRODUCT REQUIREMENT field for this product. For plasma type components, it may be appropriate to leave this field null.

PATIENT/PRODUCT REQUIREMENT Field # .09: Choices are CROSMATCH or PLASMA/PATIENT COMPATIBILITY. The entry here controls whether or not a specific component assigned to a patient must have a crossmatch interpretation of Compatible or INCOMPATIBLE, GIVE WITH BB DIRECTOR APPROVAL entered prior to relocation from the Blood Bank. If PLASMA/PATIENT COMPATIBILITY is selected, then only a check on the ABO/Rh of the patient and blood component type are made to determine if they are compatible according to standard accepted operating practices.

VOLUME (ml) Field # .1: A required field—based on the average volume for the specific component being defined.

EQUIVALENT PRODUCT Field # 9: This is a pointer field that can be used to associate an ISBT 128 product type to an existing Codabar product type. Although there is no current functionality associated with this new field, it will prove helpful in a future data conversion. When defining a new ISBT 128 product type, sites are encouraged to enter the previously defined equivalent Codabar product type (if applicable) in this field.

DAYS LEFT Field # .11: This is a number between .16 and 2557 that is used to calculate a proposed expiration date when creating this product from another in inventory. For example, a 1 entered here for a Thawed plasma product would have the software suggest an expiration date of 24 hrs in the future when using the option Disposition –not transfused [LRBLIDN] to thaw a frozen plasma product.

ANTICOAGULANT/ADDITIVE Field # .12: This is a set of codes: CPD, ACD, CPDA1 and ADSOL. When creating a pediatric component, a check is made to ensure that the parent and child component type have identical entries in this field.

COLLECTION/PREP HOURS Field # .13: This field is used by the donor module to determine if the component being created has been processed within the maximum allowable time from the date/time of collection.

MAXIMUM STORAGE DAYS Field # .135: This is the maximum storage type allowed for the specific blood component. The entry here is used to prevent an unacceptable expiration date to be assigned to a blood component when receiving a component into inventory using the option Log-in regular (invoices) [LRBLILR] or Disposition –not transfused [LRBLIDN]. It is also used when calculating the age of a unit of blood in inventory to determine if it is acceptable for Pediatric transfusion.

MODIFIED BEFORE RELEASE Field # .14: This is a yes/no field. An entry of YES is made here when the blood component must be modified before release, such as a frozen blood component, which must be thawed. If an entry of YES is entered, any units of this component type that are selected for a patient MUST be modified using the option Disposition –not transfused [LRBLIDN] prior to using the option Disposition –relocation [LRBLIDR] to issue the unit.

CAN BE REQUESTED Field # .15: This is a yes/no field. Only blood components with a YES entry in this field can be requested using options Specimen log-in [LRBLPLOGIN] or Blood component requests [LRBLPCS]. It is highly recommended that sites restrict choices by entering a NO here for any blood components not actively in use.

PATIENT SPECIMEN AGE ALLOWED Field # .16: For components that require pre-transfusion testing, a check is made to this field to determine the maximum specimen age allowable for the component. At the time of component request and selection, the current time is determined, the earliest allowable specimen date/time is calculated from the entry in this field, and the database is searched for a valid specimen.

RETYPE AFTER PREPARATION Field # .18: This is a yes/no field. Answer YES to this field if the component is prepared in the facility and must have ABO/Rh testing performed after preparation. A YES entry here will add newly created components to the Inventory ABO/Rh testing worksheet [LRBLIW] and prevent the components from being issued using the option Disposition –relocation [LRBLIDR] until ABO/Rh confirmation results are entered. When defining a blood component that will be the target component for Pediatric unit preparation [LRBLPED], the entry in this field must be YES.

CONTAINS RED BLOOD CELLS Field # .19: This is a yes/no field. If the component type contains red cells, answer YES here. A Yes here will control whether specific components are added to the Inventory ABO/Rh testing worksheet [LRBLIW], when components are received using the option Log-in regular (invoices) [LRBLILR].

MAX AGE FOR PEDIATRIC USE Field # .21: If this product can be used to prepare Pediatric Units for transfusion, enter the maximum number of days allowed from the date of collection to its use for pediatric unit preparation. The number entered here is used in conjunction with the unit expiration date and MAXIMUM STORAGE DAYS to determine whether the age of a unit is acceptable.

PEDIATRIC PRODUCT Field # .22: If the current product can be made into a Pediatric product, the entry here is the component that corresponds to the pediatric component. The entry must already exist in the BLOOD PRODUCT File (#66), the product name must contain the word PEDIATRIC (if Codabar) and the entries in the ANTICOAGULANT/ADDITIVE and IS ISBT128 fields must match. When defining this field for an ISBT 128 product type, enter the initial aliquot divided component (PRODUCT CODE α0000tA0) in this field.

SPECIFIC GRAVITY Field # .23: This is the specific gravity of the component and used to calculate the weight of a component from the volume. This calculation is done during Pediatric product preparation.

MAXIMUM INFUSION TIME(MIN) Field # .24: The number of minutes entered here is used to determine if a transfusion episode should be added to the Prolonged transfusion times [LRBLPIT] report. The date/time of transfusion completion is compared to the date/time of relocation and elapsed time is compared to the entry in this field for the component type. If the elapsed time is greater than the time entered, the transfusion episode is placed in a report queue.

AUTOLOGOUS/DIRECTED COMPONENT Field # .25: This is a yes/no field. If this specific component type is autologous or directed, answer YES here. A YES entry in this field will require that any components received during Log –in regular (invoices) [LRBLILR] be associated with a valid patient at the time of receipt. A valid patient is one who is entered in the VA PATIENT File (#2).

ADMINISTRATIVE CATEGORY Field # .26: This field consists of a set of codes to assist in defining a blood product into a specific category. The Blood Bank Administrative Data [LRBLA] report is sorted according to Administrative Categories.

POOLED PRODUCT Field # .27: This is a yes/no field.. If this product type is a pooled product, a YES must be entered here.

ASK BAG LOT Field # .28: This is a yes/no field. Enter YES here if this product is made from another in inventory and you wish to be prompted to record the bag lot # during preparation.

DESCRIPTION Field # 1: This is an optional word-processing field that can be used to enter a text description of the product.

Select SYNONYM Field # 2: : This is an optional free text field. An alternate name for a blood product up to 25 characters can be entered here. It can be used to lookup an existing entry.

Select MODIFY TO Field # 3: Multiple field. For each component type that can be made into other component types, enter the child component type in the MODIFY TO field and complete the NOT ONLY ONE ALLOWED field as applicable.

MODIFY TO Field # 66.03,.01: If this component type can be made into other component types, enter the child component type here. Prior to entry, the component type must have been previously defined as a valid entry in the BLOOD PRODUCT File and the entry for the IS ISBT128 fields must match.

NOT ONLY ONE ALLOWED Field # 66.03,.02: If more than one component type can be made from the parent, enter YES. For example, if the parent unit is whole blood, both a red cell and a plasma product can be created from it.

Select SUPPLIER Field # 4: : This is a multiple field, and at least one entry is required for each active blood component type in use at a site. How the sub-fields are defined in this section control how the UNIT ID barcode is interpreted when scanned. Depending upon your blood product supplier's practices, you may need one or many entries in this multiple field to properly interpret Codabar labeled units. The Red Cross, for example, may ship blood components all over the United States, and a SUPPLIER multiple entry should be created for each Red Cross collection facility in order for the correct eye-readable prefixes to be assigned at the time of unit log-in. In the case of the Red Cross, there is a one to one relationship between the collection facility/FDA Registration number and the eye-readable prefix, and this SUPPLIER multiple should be considered a COLLECTION FACILITY multiple. As your blood suppliers transition to ISBT 128 labeling, only one SUPPLIER multiple entry is needed for each ISBT 128 component type processed at your facility, unless you are supplied the same component type by multiple facilities and the component costs are different. However, creating multiple SUPPLIERS for the same component type allows a blood bank to track costs separately.

SUPPLIER Field # 66.01,.01: This is the free text name of the SUPPLIER/COLLECTION FACILITY.

SUPPLIER Preference number Field # 66.01,.001: This number is automatically assigned when the new SUPPLIER multiple entry is created and used internally by the software.

COST Field # 66.01,.02: This is the cost of the specific component charged by the specific supplier of the product. The number entered here is reflected in both the Supplier invoices (inventory) [RBLRIN] and Supplier transactions (inventory) [RBLRIT] reports.

ADDRESS LINE 1 Field # 66.01,.03: : This is the optional address of the supplier/collection facility

ADDRESS LINE 2 Field # 66.01,.04 :

ADDRESS LINE 3 Field # 66.01,.05: :

CITY Field # 66.01,.06: : This is the optional city of the supplier/collection facility

STATE Field # 66.01,.07: This is optional state of the supplier/collection facility

ZIP CODE Field # 66.01,.08: This is the optional zip code of the supplier/collection facility

PHONE Field # 66.01,.09: This is the optional phone number of the supplier/collection facility.

SUPPLIER PREFIX NUMBER Field # 66.01,,1: This is the eye-readable prefix that may be used by a supplier/collection facility using Codabar symbology to label units. The use of the eye-readable prefix is not consistent between all blood collection facilities, but it is consistent within a specific collection facility. If present, this is a 2-digit number that will always be appended at the beginning of the scanned Unit ID when processing units from this specific supplier during the option Log –in regular (invoices) [LRBLILR]. If the collection facility does not use an eye-readable prefix, OR if this is an ISBT 128 component type, leave this field null.

REGISTRATION NUMBER Field # 66.01,,11: This is the FDA Registration number assigned to a specific SUPPLIER/COLLECTION FACILITY. It is encoded on the lower-most right hand corner of a Codabar labeled blood bag. See Appendix A for a list of the American Red Cross Collection Facility Registration Numbers.

==>NOTE: There is no REGISTRATION NUMBER barcode on an ISBT 128 product. When defining an ISBT 128 product, leave this field null.

UNIT LABEL NON-STANDARD Field # 66.01,,12: This field is used to determine whether a Codabar-labeled unit contains alpha characters or is strictly numeric. Answer NO here if the component is labeled using Codabar and this SUPPLIER/COLLECTION FACILITY uses alpha characters in the Codabar Unit ID. If the SUPPLIER/COLLECTION FACILITY labels in Codabar using a totally numeric Unit ID OR the component is labeled using ISBT 128, enter YES here or leave NULL.

Select LOT # Field # 66.01,1: Multiple field—can be used if lot number and expiration dates of certain products are tracked.

LOT # Field # 66.02,01: This is the lot number for the specific product being tracked.

EXPIRATION DATE Field # 66.02,,02: This is the expiration date of the lot number for the specific product being tracked.

CRITERIA FOR USE Field # 66,5: This is a free text word-processing field. Can be used to document criteria for the specific blood that has been defined by the facility. This field is not currently used by the Blood Bank application but was intended for future use. However, data entry here can be viewed using FileMan to inquire to the BLOOD PRODUCT File (#66).

Select TESTS TO CHECK Field # 6: This is a multiple field that can be used to define CH Subscripted tests whose most recent results will be compared to pre-defined criteria when this blood product is ordered, either through Specimen log-in [LRBLPLOGIN] or Blood component requests [LRBLPCS], and the user answers NO to the prompt “Is patient Pre-op”. If no previous results are available, or if previous results fall outside of the criteria defined, a message is displayed stating this and override is required to continue placing an order for this blood component. Additional fields are also prompted when the product order is placed after the override. The ordering episode is captured by the system and is available on the Inappropriate transfusion requests report [LRBLPRIT], which can be printed at any time.

TESTS TO CHECK Field # 66.04,.01: Name or Abbreviation of CH Subscript test to be evaluated

SPECIMEN Field # 66.04,.02: Site/Specimen type of CH Subscript test to be evaluated

> OR < TEST VALUE Field # 66.04,.03: Value of CH Subscript test to trigger message and override. The criteria AND the value must be entered here (i.e. >8).

REQUISITION INSTRUCTIONS Field # 66.7: This is a free text word-processing field that can be used to document requisition instructions. This text is displayed if a user answers YES to the prompt FOR TRANSFUSION REQUESTS: Display instructions for components? NO// when using options Specimen log-in [LRBLPLOGIN] or Blood component requests [LRBLPCS] to place an order for components.

Select PRE-OP TESTS TO CHECK Field # 66.8: This is a multiple field that can be used to define CH Subscripted tests whose most recent results will be compared to pre-defined criteria when this blood product is ordered, either through Specimen log-in [LRBLPLOGIN] or Blood component requests [LRBLPCS], and the user answers YES to the prompt “Is patient Pre-op?”. If no previous results are available, or if previous results fall outside of the criteria defined, a message is displayed stating this and override is required to continue placing an order for this blood component. Additional fields are also prompted when the product order is placed after the override. The ordering episode is captured by the system and is available on the Inappropriate transfusion requests report [LRBLPRIT], which can be printed at any time.

PRE-OP TESTS TO CHECK Field # 66.08,.01: Name or Abbreviation of CH Subscript test to be evaluated

SPECIMEN Field # 66.08,.02: Site/Specimen type of CH Subscript test to be evaluated.

> OR < TEST VALUE Field # 66.08,.03: Value of CH Subscript test to trigger message and override. The criteria AND the value must be entered here (i.e. >45).

Select WKLD CODE Field # 66.500: This is the workload code specific to this component. An entry should be made here if this component is created in the facility, either through a donor program or through modification using the option Disposition – not transfused [LRBLIDN]. This is a multiple field.

WKLD CODE Field # 66.06,.01: This is a pointer to the WKLD CODE File (#64). The actual workload code is entered here if applicable.

Changes in Specific Options

The following section details specific changes observed in Blood Bank options after installation of LR*5.2*267.

BP Edit Blood Product File [LRBLSEB]

Following is an example of creating new entry in BLOOD PRODUCT file (#66) for an ISBT 128 labeled product. An AS-5 Red Blood Cell is used as the example.

The ISBT 128 Product Description for the product is RED BLOOD CELLS|AS-5/450mL/refr
The ISBT 128 product code is E0385V00.

The new or moved fields are underlined. User input is **bolded**.

```
BP Edit blood product file

Select BLOOD PRODUCT NAME: RED BLOOD CELLS|AS-5/450mL/refr
Are you adding 'RED BLOOD CELLS|AS-5/450mL/refr' as
a new BLOOD PRODUCT (the 125TH)? No// Y (Yes)
BLOOD PRODUCT PRODUCT CODE: E0385V00
BLOOD PRODUCT VOLUME (ml): 225
DESCRIPTION:
No existing text
Edit? NO// <cr>
BLOOD PRODUCT Select SYNONYM: AS-5 RBC
BLOOD PRODUCT Select SYNONYM: <cr>
NAME: RED BLOOD CELLS|AS-5/450mL/refr Replace <cr>
ABBREVIATION: AS-5
CAN BE MODIFIED: Y YES
IDENTIFIER: BB COMPONENT/DERIVATIVE
PRODUCT CODE: E0385V00// <cr>
IS ISBT128: Y YES (This is an ISBT128 product type)
Select ASSOCIATED DIVISION: 428 Dallas CIOFO TX CIOFO 428
Select ASSOCIATED DIVISION: <cr>
DOD CODE: <cr>
MODIFICATION CRITERIA: <cr>
PATIENT/PRODUCT ABO: 2 MUST BE COMPATIBLE
PATIENT/PRODUCT RH: 2 MUST BE COMPATIBLE
PATIENT/PRODUCT REQUIREMENT: C CROSSMATCH
VOLUME (ml): 225//<cr>
EQUIVALENT PRODUCT: <cr>
DAYS LEFT: 35
ANTICOAGULANT/ADDITIVE: ADSOL ADSOL
COLLECTION/PREP HOURS: <cr>
MAXIMUM STORAGE DAYS: 35
MODIFIED BEFORE RELEASE: <cr>
CAN BE REQUESTED: Y YES
PATIENT SPECIMEN AGE ALLOWED: 240
RETYPE AFTER PREPARATION: <cr>
CONTAINS RED BLOOD CELLS: Y YES
MAX AGE FOR PEDIATRIC USE: <cr>
PEDIATRIC PRODUCT: <cr>
```

Continued on next page...

Creating a new entry in BLOOD PRODUCT File (#66) continued

```
SPECIFIC GRAVITY: R RED BLOOD CELLS
MAXIMUM INFUSION TIME(MIN): <cr>
AUTOTOLOGOUS/DIRECTED COMPONENT: <cr>
ADMINISTRATIVE CATEGORY: RBC RBC
POOLED PRODUCT: <cr>
ASK BAG LOT #: <cr>
DESCRIPTION:
    No existing text
    Edit? NO// <cr>
Select SYNONYM: AS-5 RBC// <cr>
Select MODIFY TO: <cr>
Select SUPPLIER: ARC
    SUPPLIER Preference number: 1// <cr>
    SUPPLIER COST: 120
    COST: 120// <cr>
    ADDRESS LINE 1: <cr>
    ADDRESS LINE 2: <cr>
    ADDRESS LINE 3: <cr>
    CITY: <cr>
    STATE: <cr>
    ZIP CODE: <cr>
    PHONE: <cr>
    SUPPLIER PREFIX NUMBER: <cr>
    REGISTRATION NUMBER: <cr>
    UNIT LABEL NON-STANDARD: <cr>
    Select LOT #: <cr>
Select SUPPLIER: <cr>
CRITERIA FOR USE:
    No existing text
    Edit? NO// <cr>
Select TESTS TO CHECK: <cr>
REQUISITION INSTRUCTIONS:
    No existing text
    Edit? NO// <cr>
Select PRE-OP TESTS TO CHECK: <cr>
EQUIVALENT PRODUCT: AS-5 RED BLOOD CELLS
Select ASSOCIATED DIVISION: Dallas CIOFO// <cr>
Select WKLD CODE: <cr>
```

LR Log-in Regular (Invoices) [LRBLILR]

The option Log-in regular (invoices) [LRBLILR] is modified to accept barcode scanner input from ISBT 128 ABO/Rh, Unit ID and product code barcodes. The ability to accept barcode scanner input from the ABO/Rh, Unit ID, product code and FDA Registration # barcode from Codabar labeled units as well as manual data entry remains unchanged.

Highlights of changes observed as a result of installation of patch LR*5.2*267:

Prior to this patch, when a barcode is scanned at prompts designed to accept scanner input, the screen echoes what the scanner literally reads and then displays the interpretation. After installation of this patch, the users may notice that the echo of the scanned input may display for a split second and be erased prior to the display of the interpretation. This is normal and intentional. Users will notice this split-second display-erase-redisplay for any data input at prompts that are designed to accommodate barcode data input, including manual data entry.

Workflow changes once your supplier begins transition to ISBT 128 labeled products

Sites may have created several SUPPLIER multiple entries for each blood product defined in the BLOOD PRODUCT File (#66) in order to accommodate multiple UNIT ID formats (multiple prefixes, numeric vs. alpha characters etc.). In addition, sites may have populated the REGISTRATION NUMBER Field (#66.01,.11) within the SUPPLIER multiple in order to scan the Codabar FDA Registration Number barcode to populate the SUPPLIER prompt when logging in units using this option. This practice will not be necessary when using the ISBT 128 system if the site has a single source for their blood products.

The ISBT 128 system has a consistent format for the structure of the Unit ID barcode, therefore, only a single entry in the SUPPLIER multiple for each component processed should be necessary in order to properly interpret the Unit ID barcode.

A situation that could require multiple SUPPLIER entries for an ISBT 128 blood product is the case where there is more than one source for the blood component. This could be the case in a multidivisional institution. In order to have accurate Blood inventory transaction reports [LRBLITX] and Supplier transactions (inventory) [LRBLRIT] it may be necessary to create multiple SUPPLIER entries for an ISBT 128 blood product.

An example of what is seen during processing of a shipment of ISBT 128 components after installation of LR*5.2*267 follows. A barcode scanner is used to scan ISBT 128 ABO/RH, Unit ID and Expiration date barcodes.

```
Select Inventory Option: LR Log-in regular (invoices)

                                Blood Component Log-In

Division: Dallas CIOFO

To use BAR CODE READER
Pass reader wand over a GROUP-TYPE (ABO/Rh) label
=> (bar code) A NEG

Enter INVOICE (or order) NUMBER: EXAMPLE1
DATE/TIME RECEIVED: NOW// (MAR 21, 2001@11:11)

Invoice number: EXAMPLE1
Select BLOOD COMPONENT: (Bar code)
                    RED BLOOD CELLS|AS-5/450mL/refr
E0385V00      AS-5      1
Select SUPPLIER: ARC// <CR>      120

UNIT ID: (Bar code) UNIT ID: W001399000168
ABO/Rh: (Bar code) ABO/Rh: A NEG
EXPIRATION DATE/TIME: (Bar code) Exp date: Apr 20, 2001 23:59 (APR 20, 2001@23:59)

UNIT ID:

RED BLOOD CELLS|AS-5/450mL/ref Source: ARC Invoice: EXAMPLE1
Review: Unit          ABO/Rh   Expiration date (*=Expired or expires today)
1)      W001399000168   A NEG    Apr 20, 2001 23:59

All OK ? YES// (YES)

Invoice number: EXAMPLE1
Select BLOOD COMPONENT:
```

DN Disposition – Not Transfused [LRBLIDN]

The option Disposition –not transfused [LRBLIDN] is modified to accept barcode data input from an ISBT 128 Unit ID barcode. The ability to accept barcode data input from a Codabar Unit ID barcode as well as manual data entry remains unchanged. Changes in the logic used to create divided units from an ISBT 128 product type are included in this patch.

Highlights of changes observed as a result of installation of patch LR*5.2*267:

Prior to using this option to modify an ISBT 128 product into divided products, sites must create unique entries in the BLOOD PRODUCT File (#66) equal to the number of aliquots to be prepared. The PRODUCT CODE Field (#66,.05) for these new entries must be defined using the first six (6) characters of the parent unit, then appending A0, B0, C0, etc. for characters 7-8 for each divided product created.

The main differences between dividing a Codabar and an ISBT 128 product type are as follows:

Codabar: For each aliquot prepared, the system assigns a Unit ID the same as a parent to which it appends the letters A, B, C etc. to identify the specific aliquot. A single entry in the BLOOD PRODUCT File (#66) defining a Divided Unit is required.

ISBT 128: For each aliquot prepared, the system assigns a Unit ID that is identical to the parent. The system also searches the BLOOD PRODUCT File (#66) for entries in the BLOOD PRODUCT File (#66) that have a PRODUCT CODE Field (#66,.05) defined using the first 6 characters of the parent unit and A0, B0, C0 for characters 7-8 etc. for the total number of aliquots requested. If inadequate entries exist in the BLOOD PRODUCT File (#66) to process the number of aliquots requested, the system displays a warning message.

NOTE: When populating the MODIFY TO field (#66.03,.01) for an ISBT 128 product that CAN be processed into divided units, enter the divided component that indicates the ExxxxxA0 product code only. Do NOT enter each possible aliquot product created in this field.

The following table illustrates the main differences between dividing a Codabar and an ISBT 128 product type.

Example: Expected outcomes of dividing blood components using Disposition –not transfused [LRBLIDN].

Product Type	Parent Unit ID	Divided Unit ID	Component Name	Product Code
Codabar	04FK54321		AS-1 RED BLOOD CELLS	04210
		04FK54321A	AS-1 DIVIDED RED BLOOD CELLS	Product Code is optional
		04FK54321B	AS-1 DIVIDED RED BLOOD CELLS	Product Code is optional
		04FK54321C	AS-1 DIVIDED RED BLOOD CELLS	Product Code is optional
ISBT 128	W001312345678		ISBT 128 AS-1 RBC	E0291000
		W001312345678	ISBT 128 AS-1 RBC Split A	E02910A0 (Required)
		W001312345678	ISBT 128 AS-1 RBC Split B	E02910B0 (Required)
		W001312345678	ISBT 128 AS-1 RBC Split C	E02910C0 (Required)

Example: Using Disposition -not transfused [LRBLIDN] to create divided units from an ISBT 128 product type.

The following example demonstrates the use of Disposition –not transfused [LRBLIDN] to create two (2) divided units from an ISBT 128 product type. User input is in **bold**. Note that in the screen capture, three (3) aliquots are originally requested, demonstrating the error message that is displayed when inadequate entries exist in the BLOOD PRODUCT File (#66) for the number of aliquots requested.

Three separate entries in the BLOOD PRODUCT File (#66) have been previously defined to create this example. Key field definitions for creating these blood products are detailed in the following table:

Product NAME	Product Code	MODIFY TO:
RED BLOOD CELLS AS-5/450mL/refr	E0385V00	RED BLOOD CELLS AS-5 Divided A
RED BLOOD CELLS AS-5 Divided A	E0385VA0	
RED BLOOD CELLS AS-5 Divided B	E0385VB0	

```
Select Inventory Option: DN Disposition -not transfused
Division: Dallas CIOFO
To use BAR CODE READER
Pass reader wand over a GROUP-TYPE (ABO/Rh) label
=> (bar code) A POS

Select UNIT ID FOR DISPOSITION: (Bar code)UNIT ID: W001399000168      ANEG  RED B
LOOD CELLS|AS-5/450mL/refr      RED BLOOD CELLS|AS-5/450mL/refr      NEG    A NEG
RED BLOOD CELLS|AS-5/450mL/refr
DISPOSITION: MODIFY
DISPOSITION DATE: NOW// <cr> (MAR 23, 2001@09:34)
VOLUME (ml): 225//
Select MODIFY TO: RED BLOOD CELLS|AS-5 Divided A      E0385VA0      AS5A      0
Enter number of aliquots (1-5): 3
1 MORE DIVIDED BLOOD PRODUCT ENTRY MUST BE CREATED BEFORE THE PRODUCT
TYPE YOU HAVE SELECTED CAN BE SPLIT INTO 3 UNITS.
Enter number of aliquots (1-5): 2

New ID #: W001399000168 RED BLOOD CELLS|AS-5 Divided A
DATE/TIME RECEIVED: NOW// (MAR 23, 2001@09:34)
EXPIRATION DATE/TIME: Mar 24, 2001@0934// <cr> (MAR 24, 2001@09:34)

New ID #: W001399000168 RED BLOOD CELLS|AS-5 Divided B
DATE/TIME RECEIVED: NOW// (MAR 23, 2001@09:34)
EXPIRATION DATE/TIME: Mar 24, 2001@0934// <cr> (MAR 24, 2001@09:34)

Select UNIT ID FOR DISPOSITION:
```

PD Pediatric Unit Preparation [LRBLPED]

The option Pediatric unit preparation [LRBLPED] is modified to accept barcode data input from ISBT 128 Unit ID and ISBT 128 product code barcodes. The ability to accept barcode data input from Codabar Unit ID and Codabar product code barcodes, as well as manual data entry, remains unchanged. Changes in the logic used to create pediatric aliquots from an ISBT 128 product type are included.

Highlights of changes observed as a result of installation of patch LR*5.2*267:

Prior to using this option to create pediatric aliquots from an ISBT 128 product, sites must create unique entries in the BLOOD PRODUCT File (#66) equal to the number of aliquots to be prepared. The PRODUCT CODE Field (#66,.05) for these new entries must be defined using the first six (6) characters of the parent unit, then appending A0, B0, C0, etc. for characters 7-8 for each pediatric product created.

The main differences between dividing a Codabar and an ISBT 128 product type are as follows:

Codabar: For each aliquot prepared, the system assigns a Unit ID the same as a parent to which to which it appends the letters PA, PB, PC etc. to identify the specific aliquot. A single entry in the BLOOD PRODUCT File (#66) defining a PEDIATRIC product is required. The word PEDIATRIC must be included in the NAME field (#66,.01) for the pediatric product.

ISBT 128: For each aliquot prepared, the system assigns a unit ID that is identical to the parent. When a pediatric aliquot is created from an ISBT 128 unit, the system searches to see how many previous aliquots have been prepared. The system then searches the BLOOD PRODUCT File (#66) to see if there is an entry with the next logical PRODUCT CODE assigned. The word PEDIATRIC does NOT need to be included in the blood product name. Sites that create both pediatric aliquots and divide units prior to transfusion will use the same Divided product entries as the aliquot units.

NOTE: The Retype After Preparation field in the BLOOD PRODUCT File (#66) must be set to YES for each child product type created.

NOTE: When populating the PEDIATRIC PRODUCT field (#66,.22) for an ISBT 128 product that CAN be processed into pediatric aliquots, enter the divided component that indicates the ExxxxxA0 product code. Any additional aliquot products must exist, however, they do not need to be associated with the parent component type in order to prepare the pediatric preparations.

The following table illustrates the main differences between creating pediatric aliquots from a Codabar and an ISBT 128 product type.

Example: Expected outcomes of creating pediatric aliquots using the option Pediatric Unit Preparation [LRBLPED].

Product Type	Parent Unit ID	Pediatric Aliquot Unit ID	Component Name	Product Code
Codabar	04FK54321		AS-1 RED BLOOD CELLS	04210
		04FK54321PA	AS-1 PEDIATRIC RED BLOOD CELLS	Product Code is optional
		04FK54321PB	AS-1 PEDIATRIC RED BLOOD CELLS	Product Code is optional
		04FK54321PC	AS-1 PEDIATRIC RED BLOOD CELLS	Product Code is optional
ISBT 128	W001312345678		ISBT 128 AS-1 RBC	E0291000
		W001312345678	ISBT 128 AS-1 RBC Split A	E02910A0 (Required)
		W001312345678	ISBT 128 AS-1 RBC Split B	E02910B0 (Required)
		W001312345678	ISBT 128 AS-1 RBC Split C	E02910C0 (Required)

The following is a screen capture of the option Pediatric Unit Preparation [LRBLPED] using an ISBT 128 product type. This example demonstrates the first pediatric aliquot to be prepared.

```
Select Inventory Option: PD  Pediatric unit preparation
Division: Dallas CIOFO
To use BAR CODE READER
Pass reader wand over a GROUP-TYPE (ABO/Rh) label
=> (bar code) A POS

Blood component for pediatric prep: (Bar code)
RED BLOOD CELLS|AS-5/450mL/refr      E0385V00      AS-5
1

Select UNIT: (Bar code)UNIT ID: W001399000220  W001399000220
W001399000220 A NEG 04/27/01 <1 DAY OLD 225 ml

W001399000220      A NEG 04/27/01 Vol(ml): 225 Wt(gm): 243
VOL('W' to edit weight, 'V' to edit volume): 225ml//

Enter volume(ml) for pediatric unit: 10

W001399000220 A NEG vol(ml):10 <cr>
Expiration date: T@2359 (MAR 23, 2001@23:59)

OK to process pediatric unit ? NO// Y (YES)

Date/time work completed: NOW// <cr> (MAR 23, 2001@10:09)

Blood component for pediatric prep:
```

The following is a screen capture of an attempt to create a pediatric aliquot and the system determines that additional entries are needed in the BLOOD PRODUCT File (#66) to create the aliquot.

```
Select Inventory Option: Pediatric unit preparation
Division: Dallas CIOFO
To use BAR CODE READER
Pass reader wand over a GROUP-TYPE (ABO/Rh) label
=> (bar code) A NEG

Blood component for pediatric prep: (Bar code)
RED BLOOD CELLS|AS-5/450mL/refr      E0385V00      AS-5
1

Select UNIT: (Bar code)UNIT ID: W001399000220  W001399000220

Pediatric Preparation cannot proceed with this unit until another
record is created for this product type in the BLOOD PRODUCT file.

Select UNIT:
```

Additional Options Modified

Options Modified to Accept Barcode Scanner Input for an ISBT 128 Unit ID Barcode

The following options have been modified to accept barcode scanner input from an ISBT 128 Unit ID barcode label. The ability to accept barcode data input from a Codabar Unit ID barcode as well as manual data entry remains unchanged.

- Unit ABO/Rh confirmation [LRBLIUC] (By individual unit ID)
- Select Units for Patients [LRBLPIC]
- Edit pooled blood product [LRBLJM]

Options Modified to Accept Manual Data Input of a 13 Character ISBT 128 Unit ID

The following options have been modified to accept manual data entry of the longer Unit ID seen with ISBT 128 products.

- Enter blood inventory typing charges [LRBLILS]
- Unit phenotyping [LRBLIUP]
- Edit unit disposition fields [LRBLSED]
- Edit unit log-in [LRBLSEL]
- Edit unit - patient fields [LRBLSEC]
- Free autologous/directed donor units [LRBLSEE]
- Single unit status [LRBLQST]
- Single unit information- display [LRBLIPSD]
- Single unit information- print [LRBLIPSP]
- Special typing charges (inventory) [LRBLRIS] (edit individual unit)

Options and Reports Modified to Print and/or Display the Longer ISBT 128 Unit ID

The following options and reports have been modified to accommodate the longer Unit ID seen with ISBT 128 products:

- Inventory ABO/Rh testing worksheet [LRBLIW]
- Unit ABO/Rh Confirmation [LRBLIUC] (By invoice)
- Blood component requests [LRBLPCS]
- Enter crossmatch results [LRBLPX]
- Unit CAUTION tag labels [LRBLILA]
- Disposition – Relocation [LRBLIDR]
- Blood transfusion results [LRBLPT]
- Shipping invoices for blood components [LRBLISH]
- Units release to stock (cancel) by patient [LRBLIUR]
- Units assigned/components requested [LRBLQPR]
- Print single BB patient report [LRBLP PRINT SINGLE]
- Blood bank consultation reports [LRBLCN]
- CMV Antibody Status Report [LRBLICV]
- Disposition-not transfused [LRBLIDU]
- Units available (indate/no disposition) [LRBLRUA]
- Units with no disposition [LRBLRUN]
- Units on Xmatch by date/time xmatched [LRBLIX]
- Supplier invoices (inventory) [LRBLRIN]
- Special typing charges (inventory) [LRBLRIS] (report)
- Supplier transactions (inventory) [LRBLRIT]
- Phenotyped units available [LRBLIPH]
- Crossmatch/Transfusions by Specialty/Physician [LRBLAA] (detailed)
- Crossmatch:Transfusion report [LRBLRCT]
- Unit issue book entries [LRBLIRB]
- Prolonged transfusion times [LRBLPIT]
- Transfusion data report [LRBLITR]
- Transfusions by treating specialty/physician [LRBLITS]
- Print data change audits [LRBLAD]
- Print units with final disposition [LRBLRUF]
- Patient blood bank record [LRBLQDR]
- Units assigned/components requested [LRBLQPR]

Appendix A - Supplier Multiple Entries for ARC

To properly interpret the UNIT ID for blood components provided by the American Red Cross (ARC), multiple entries should be created in the SUPPLIER multiple to reflect each eye-readable prefix supplied for each blood component provided by your ARC. If your local ARC imports blood from other ARC regions, it may be necessary to enter most or all of the available ARC prefixes. It is recommended that you create these entries now, rather than as needed.

Below is a list of the ARC suppliers and the relevant information for the minimum fields, in addition to COST (required), which should be defined for each ARC entry:

AMERICAN RED CROSS (ARC) SUPPLIER NAME	SUPPLIER PREFIX NUMBER	REGISTRATION NUMBER	UNIT LABEL NON-STANDARD
Alabama	41	110730011	NO
Appalachian	35	111730101	NO
Arizona	07	120729971	NO
Badger-Hawkeye	32	121730281	NO
Carolinas	12	110730071	NO
Central Ohio	16	115730131	NO
Central Plains	02	119730421	NO
Connecticut	33	112730141	NO
Great Lakes	18	118730331	NO
Greater Alleghenies	27	125730161	NO
Greater Chesapeake and Potomac	53	111730111	NO
Greater Ozarks-Arkansas	55	123729981	NO
Gulf Coast	26	110730051	NO
Heart of America	40	114730431	NO
Indiana-Ohio	38	118730311	NO
Lewis and Clark	20	130729901	NO
Mid-Atlantic	29	111730241	NO
Midwest	09	119730371	NO
Missouri-Illinois	11	119730351	NO
New England	04	112700261	NO
New York-Penn	01	124384451	NO
North Central	17	121730381	NO
Northeastern Penn	30	125730181	NO
Northern California	08	129714301	NO
Northern Ohio	42	115730191	NO
Pacific Northwest	21	130729961	NO
Penn-Jersey	22	125730211	NO
Puerto Rico	54	126759451	NO
River Valley	24	110730031	NO
South Carolina	36	110730091	NO
Southeastern Michigan	13	118730441	NO
Southern	03	110730001	NO
Southern California	06	120729941	NO
Southwest	49	116730401	NO
Tennessee Valley	19	110730061	NO
Western Lake Erie	50	115730201	NO

Appendix B - US ISBT 128 Product Codes

This document contains the PRODUCT DESCRIPTION (Name) and the 5-digit ISBT product code of ISBT 128 blood products approved for use in the US as of March 1, 2001. The Product Description and Product Code fields have been extracted from a database provided by the International Council for Commonality in Blood Banking Automation, Inc.

The Product Description field reflects the proper name assigned to the blood component using the ISBT 128 labeling standard. It follows the format of:

Blood Component|Core Condition|Other Attributes|Other Attributes

See Section ISBT 128 BARCODE CHARACTERISTICS FOR U.S. IMPLEMENTATION, heading Structure of ISBT 128 Blood Product Description contained earlier in this ISBT 128 implementation guide for a detailed explanation of the structure of these product description names.

The Product Code field in this table reflects the random 5-digit code assigned to a specific product type. Products that are received from an outside facility will have an additional three digits appended to this code. The sixth character will vary depending upon the type of collection (the default is zero ("0") and characters 7-8 are usually zero ("0") when received from an outside collection facility.

This table should be used as a reference when creating new entries in the BLOOD PRODUCT File (#66) for ISBT 128 products that are created as a result modification of an existing ISBT 128 product from inventory or collected by your facility. When creating new entries in the BLOOD PRODUCT File for an ISBT 128 component type, the 5-digit code provided in the table below should be appended with three zeros ("0") at the end.

An example would be:

If your blood supplier provides you with the Fresh Frozen Plasma type FRESH FROZEN PLASMA|CP2D/XX/<=18C the product code would be E0713000.

In order to process the frozen unit into a thawed component, an entry in the BLOOD PRODUCT File (#66) should be created for Thawed FRESH FROZEN PLASMA|CP2D/XX/refg. The table below lists the 5-digit code as E0797. In the BLOOD PRODUCT File entry for this thawed component, enter the PRODUCT CODE as E0797000.

<u>Product Description</u>	<u>Product Code</u>
APHERESIS CRYOPRECIPITATE None/XX/<=-18C.....	E3597
APHERESIS CRYOPRECIPITATE None/XX/<=-18C Irradiated.....	E3598
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C.....	E0869
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C <200 mL.....	E0898
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C >=200 mL <400mL	E0900
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C >=400mL <600mL	E0902
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C >=600mL.....	E0904
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Aphr not automated	E0906
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C For mnf:injectable Frozen <=6h.....	E3878
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C For mnf:noninjectable Frozen <=6h.....	E3881
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Frozen <=24h	E3932
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Frozen <=6h.....	E3875
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Irradiated	E0878
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Irradiated <200 mL.....	E0883
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Irradiated >=200 mL <400mL	E0885
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Irradiated >=400mL <600mL	E0887
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Irradiated >=600mL.....	E0889
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Irradiated Aphr not automated	E0891
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Irradiated Frozen <=6h.....	E3884
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Irradiated ResLeu:<1log6 Frozen <=6h	E3890
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Not for tx or mnf	E0870
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C Not for tx or mnf Aphr not automated.....	E0875
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<=-18C ResLeu:<1log6 Frozen <=6h	E3887
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-25 ResLeu:<1log6 Frozen <=6h	E3888

<u>Product Description</u>	<u>Product Code</u>
----------------------------	---------------------

APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-25C.....	E3893
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-25C For mnf:injectable Frozen <=24h.....	E3933
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-25C For mnf:injectable Frozen <=6h	E3879
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-25C For mnf:noninjectable Frozen <=6h	E3882
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-25C Frozen <=6h.....	E3876
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-25C Irradiated Frozen <=6h.....	E3885
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-25C Irradiated ResLeu:<1log6 Frozen <=6h	E3891
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C/<-30C For mnf:noninjectable Frozen <=6h	E3883
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C>=600mL Frozen <=6h 2nd container	E3945
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C>=600mL Frozen <=6h 3rd	E3994
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C For mnf:injectable >=600mL Frozen	E3944
<=6h 2nd container Quar:>=4m/retested	
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C For mnf:injectable Frozen <=24h	E3934
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C For mnf:injectable Frozen <=6h.....	E3880
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C Frozen <=6h.....	E3877
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C Irradiated Frozen <=6h.....	E3886
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C Irradiated ResLeu:<1log6 Frozen <=6h	E3892
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-30C ResLeu:<1log6 Frozen <=6h	E3889
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C.....	E1029
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C <200 mL.....	E1058
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C>=200 mL <400mL	E1060
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C>=400mL <600mL	E1062
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C>=600mL.....	E1064
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C Aphr not automated	E1066
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C Irradiated	E1038
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C Irradiated <200 mL.....	E1043
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C Irradiated >=200 mL <400mL	E1045
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C Irradiated >=400mL <600mL	E1047
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C Irradiated >=600mL.....	E1049
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C Irradiated Aphr not automated	E1051
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C Not for tx or mnf	E1030
APHERESIS FRESH FROZEN PLASMA ACD-A/XX/<-65C Not for tx or mnf Aphr not automated	E1035
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C	E0829

<u>Product Description</u>	<u>Product Code</u>
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C <200 mL.....	E0858
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C >=200 mL <400mL	E0860
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C >=400mL <600mL	E0862
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C >=600mL.....	E0864
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C Aphr not automated	E0866
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C Irradiated.....	E0838
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C Irradiated <200 mL.....	E0843
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C Irradiated >=200 mL <400mL	E0845
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C Irradiated >=400mL <600mL	E0847
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C Irradiated >=600mL.....	E0849
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C Irradiated Aphr not automated	E0851
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C Not for tx or mnf	E0830
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<=-18C Not for tx or mnf Aphr not automated.....	E0835
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C	E1069
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C <200 mL	E1098
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C >=200 mL <400mL	E1100
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C >=400mL <600mL	E1102
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C >=600mL	E1104
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C Aphr not automated	E1106
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C Irradiated	E1078
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C Irradiated <200 mL	E1083
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C Irradiated >=200 mL <400mL	E1085
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C Irradiated >=400mL <600mL	E1087
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C Irradiated >=600mL	E1089
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C Irradiated Aphr not automated	E1091
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C Not for tx or mnf.....	E1070
APHERESIS FRESH FROZEN PLASMA ACD-B/XX/<-65C Not for tx or mnf Aphr not automated	E1075
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<=-18C.....	E4015
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<=-18C/For mnf:injectable.....	E4016
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<=-18C/For mnf:noninjectable.....	E4017

<u>Product Description</u>	<u>Product Code</u>
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<=-18C/Not for tx or mnf	E4018
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<-25 C.....	E4019
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<-25 C/For mnf:injectable.....	E4020
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<-25 C/For mnf:noninjectable	E4021
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<-25 C/Not for tx or mnf	E4022
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<-30C.....	E4023
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<-30C/For mnf:injectable.....	E4024
APHERESIS FRESH FROZEN PLASMA CPD 50/XX/<-30C/For mnf:noninjectable	E4025
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C	E0909
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C <200 mL.....	E0938
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C >=200 mL <400mL.....	E0940
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C >=400mL <600mL	E0942
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C >=600mL	E0944
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C Aphr not automated.....	E0946
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C Irradiated	E0918
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C Irradiated <200 mL.....	E0923
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C Irradiated >=200 mL <400mL.....	E0925
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C Irradiated >=400mL <600mL	E0927
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C Irradiated >=600mL	E0929
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C Irradiated Aphr not automated.....	E0931
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C Not for tx or mnf	E0910
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<=-18C Not for tx or mnf Aphr not automated	E0915
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C.....	E1109
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C <200 mL	E1138
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C >=200 mL <400mL	E1140
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C >=400mL <600mL	E1142
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C >=600mL.....	E1144
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C Aphr not automated	E1146
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C Irradiated.....	E1118

<u>Product Description</u>	<u>Product Code</u>
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C Irradiated <200 mL	E1123
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C Irradiated >=200 mL <400mL	E1125
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C Irradiated >=400mL <600mL	E1127
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C Irradiated >=600mL.....	E1129
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C Irradiated Aphr not automated	E1131
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C Not for tx or mnf	E1110
APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/<-65C Not for tx or mnf Aphr not automated.....	E1115
APHERESIS FRESH FROZEN PLASMA NS/XX/<-30C >=200 mL<400mL	E3828
APHERESIS FRESH FROZEN PLASMA NS/XX/<-30C >=400mL<600mL	E3827
APHERESIS FRESH FROZEN PLASMA NS/XX/<-30C ResLeu:<5log6	E4004
APHERESIS FRESH FROZEN PLASMA NS/XX/<-30C ResLeu:<5log6 >=200 mL <400mL	E4008
APHERESIS GRANULOCYTES/PLATELETS NaCitrate-HES/XX/rt.....	E3691
APHERESIS GRANULOCYTES/PLATELETS NaCitrate-HES/XX/rt Irradiated.....	E3696
APHERESIS GRANULOCYTES/PLATELETS NaCitrate-HES/XX/rt Not for tx or mnf.....	E3692
APHERESIS GRANULOCYTES/PLATELETS NaCitrate-HES/XX/rt Not for tx or mnf Open	E3693
APHERESIS GRANULOCYTES/PLATELETS NaCitrate-HES/XX/rt Open.....	E3694
APHERESIS GRANULOCYTES/PLATELETS NaCitrate-HES/XX/rt Open Irradiated	E3695
APHERESIS GRANULOCYTES NaCitrate-HES/XX/rt	E3673
APHERESIS GRANULOCYTES NaCitrate-HES/XX/rt Irradiated	E3678
APHERESIS GRANULOCYTES NaCitrate-HES/XX/rt Not for tx or mnf	E3674
APHERESIS GRANULOCYTES NaCitrate-HES/XX/rt Not for tx or mnf Open.....	E3675
APHERESIS GRANULOCYTES NaCitrate-HES/XX/rt Open	E3676
APHERESIS GRANULOCYTES NaCitrate-HES/XX/rt Open Irradiated	E3677
APHERESIS LEUKOCYTES ACD-A/XX/refg	E3757
APHERESIS LEUKOCYTES ACD-A/XX/refg For mnf:injectable	E3758
APHERESIS LEUKOCYTES ACD-A/XX/refg For mnf:injectable Open.....	E3759
APHERESIS LEUKOCYTES ACD-A/XX/refg For mnf:noninjectable	E3760
APHERESIS LEUKOCYTES ACD-A/XX/refg For mnf:noninjectable Open	E3761
APHERESIS LEUKOCYTES ACD-A/XX/refg Not for tx or mnf	E3762
APHERESIS LEUKOCYTES ACD-A/XX/refg Not for tx or mnf Open	E3763

<u>Product Description</u>	<u>Product Code</u>
APHERESIS LEUKOCYTES ACD-A/XX/refg Open.....	E3764
APHERESIS LEUKOCYTES ACD-A/XX/rt.....	E3773
APHERESIS LEUKOCYTES ACD-A/XX/rt Aphr not automated	E3788
APHERESIS LEUKOCYTES ACD-A/XX/rt For mnf:injectable.....	E3774
APHERESIS LEUKOCYTES ACD-A/XX/rt For mnf:injectable Aphr not automated	E3777
APHERESIS LEUKOCYTES ACD-A/XX/rt For mnf:injectable Open	E3775
APHERESIS LEUKOCYTES ACD-A/XX/rt For mnf:injectable Open Aphr not automated.....	E3776
APHERESIS LEUKOCYTES ACD-A/XX/rt For mnf:noninjectable	E3778
APHERESIS LEUKOCYTES ACD-A/XX/rt For mnf:noninjectable Aphr not automated.....	E3781
APHERESIS LEUKOCYTES ACD-A/XX/rt For mnf:noninjectable Open	E3779
APHERESIS LEUKOCYTES ACD-A/XX/rt For mnf:noninjectable Open Aphr not automated.....	E3780
APHERESIS LEUKOCYTES ACD-A/XX/rt Not for tx or mnf	E3782
APHERESIS LEUKOCYTES ACD-A/XX/rt Not for tx or mnf Aphr not automated.....	E3785
APHERESIS LEUKOCYTES ACD-A/XX/rt Not for tx or mnf Open	E3783
APHERESIS LEUKOCYTES ACD-A/XX/rt Not for tx or mnf Open Aphr not automated.....	E3784
APHERESIS LEUKOCYTES ACD-A/XX/rt Open	E3786
APHERESIS LEUKOCYTES ACD-A/XX/rt Open Aphr not automated	E3787
APHERESIS LEUKOCYTES ACD-B/XX/rt	E3789
APHERESIS LEUKOCYTES ACD-B/XX/rt Aphr not automated	E3804
APHERESIS LEUKOCYTES ACD-B/XX/rt For mnf:injectable.....	E3790
APHERESIS LEUKOCYTES ACD-B/XX/rt For mnf:injectable Aphr not automated	E3793
APHERESIS LEUKOCYTES ACD-B/XX/rt For mnf:injectable Open	E3791
APHERESIS LEUKOCYTES ACD-B/XX/rt For mnf:injectable Open Aphr not automated.....	E3792
APHERESIS LEUKOCYTES ACD-B/XX/rt For mnf:noninjectable	E3794
APHERESIS LEUKOCYTES ACD-B/XX/rt For mnf:noninjectable Aphr not automated.....	E3797
APHERESIS LEUKOCYTES ACD-B/XX/rt For mnf:noninjectable Open	E3795
APHERESIS LEUKOCYTES ACD-B/XX/rt For mnf:noninjectable Open Aphr not automated.....	E3796
APHERESIS LEUKOCYTES ACD-B/XX/rt Not for tx or mnf	E3798
APHERESIS LEUKOCYTES ACD-B/XX/rt Not for tx or mnf Aphr not automated.....	E3801
APHERESIS LEUKOCYTES ACD-B/XX/rt Not for tx or mnf Open	E3799

<u>Product Description</u>	<u>Product Code</u>
APHERESIS LEUKOCYTES ACD-B/XX/rt Not for tx or mnf Open Aphr not automated	E3800
APHERESIS LEUKOCYTES ACD-B/XX/rt Open	E3802
APHERESIS LEUKOCYTES ACD-B/XX/rt Open Aphr not automated	E3803
APHERESIS LEUKOCYTES NaCitrate/XX/refg	E3765
APHERESIS LEUKOCYTES NaCitrate/XX/refg For mnf:injectable	E3766
APHERESIS LEUKOCYTES NaCitrate/XX/refg For mnf:injectable Open	E3767
APHERESIS LEUKOCYTES NaCitrate/XX/refg For mnf:noninjectable	E3768
APHERESIS LEUKOCYTES NaCitrate/XX/refg For mnf:noninjectable Open.....	E3769
APHERESIS LEUKOCYTES NaCitrate/XX/refg Not for tx or mnf.....	E3770
APHERESIS LEUKOCYTES NaCitrate/XX/refg Not for tx or mnf Open.....	E3771
APHERESIS LEUKOCYTES NaCitrate/XX/refg Open	E3772
APHERESIS LEUKOCYTES NS/XX/rt.....	E3829
APHERESIS LEUKOCYTES NS/XX/rt Irradiated.....	E3830
APHERESIS PLASMA ACD-A/XX/<=-18C.....	E1521
APHERESIS PLASMA ACD-A/XX/<=-18C <200 mL	E1600
APHERESIS PLASMA ACD-A/XX/<=-18C <200 mL Aphr not automated	E1605
APHERESIS PLASMA ACD-A/XX/<=-18C <200 mL Frozen <=24h.....	E1601
APHERESIS PLASMA ACD-A/XX/<=-18C <200 mL Frozen <=24h Aphr not automated	E1602
APHERESIS PLASMA ACD-A/XX/<=-18C <200 mL Frozen >24h	E1603
APHERESIS PLASMA ACD-A/XX/<=-18C <200 mL Frozen >24h Aphr not automated	E1604
APHERESIS PLASMA ACD-A/XX/<=-18C >=200 mL <400mL	E1606
APHERESIS PLASMA ACD-A/XX/<=-18C >=200 mL <400mL Aphr not automated	E1611
APHERESIS PLASMA ACD-A/XX/<=-18C >=200 mL <400mL Frozen <=24h	E1607
APHERESIS PLASMA ACD-A/XX/<=-18C >=200 mL <400mL Frozen <=24h Aphr not automated	E1608
APHERESIS PLASMA ACD-A/XX/<=-18C >=200 mL <400mL Frozen >24h	E1609
APHERESIS PLASMA ACD-A/XX/<=-18C >=200 mL <400mL Frozen >24h Aphr not automated	E1610
APHERESIS PLASMA ACD-A/XX/<=-18C >=400mL <600mL	E1612
APHERESIS PLASMA ACD-A/XX/<=-18C >=400mL <600mL Aphr not automated.....	E1617
APHERESIS PLASMA ACD-A/XX/<=-18C >=400mL <600mL Frozen <=24h	E1613
APHERESIS PLASMA ACD-A/XX/<=-18C >=400mL <600mL Frozen <=24h Aphr not automated	E1614

Product Description

Product Code

APHERESIS PLASMA ACD-A/XX/<=-18C >=400mL <600mL Frozen >24h	E1615
APHERESIS PLASMA ACD-A/XX/<=-18C >=400mL <600mL Frozen >24h Aphr not automated.....	E1616
APHERESIS PLASMA ACD-A/XX/<=-18C >=600mL.....	E1618
APHERESIS PLASMA ACD-A/XX/<=-18C >=600mL Aphr not automated	E1623
APHERESIS PLASMA ACD-A/XX/<=-18C >=600mL Frozen <=24h.....	E1619
APHERESIS PLASMA ACD-A/XX/<=-18C >=600mL Frozen <=24h Aphr not automated	E1620
APHERESIS PLASMA ACD-A/XX/<=-18C >=600mL Frozen >24h	E1621
APHERESIS PLASMA ACD-A/XX/<=-18C >=600mL Frozen >24h Aphr not automated	E1622
APHERESIS PLASMA ACD-A/XX/<=-18C Aphr not automated	E1628
APHERESIS PLASMA ACD-A/XX/<=-18C Frozen <=24h.....	E1624
APHERESIS PLASMA ACD-A/XX/<=-18C Frozen <=24h Aphr not automated	E1625
APHERESIS PLASMA ACD-A/XX/<=-18C Frozen >24h	E1626
APHERESIS PLASMA ACD-A/XX/<=-18C Frozen >24h Aphr not automated	E1627
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated.....	E1558
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated <200 mL	E1565
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated <200 mL Aphr not automated	E1570
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated <200 mL Frozen <=24h.....	E1566
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated <200 mL Frozen <=24h Aphr not automated	E1567
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated <200 mL Frozen >24h	E1568
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated <200 mL Frozen >24h Aphr not automated	E1569
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=200 mL <400mL	E1571
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=200 mL <400mL Aphr not automated	E1576
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=200 mL <400mL Frozen <=24h	E1572
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=200 mL <400mL Frozen <=24h Aphr not	E1573
automated	
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=200 mL <400mL Frozen >24h	E1574
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=200 mL <400mL Frozen >24h Aphr not	E1575
automated	
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=400mL <600mL	E1577
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=400mL <600mL Aphr not automated.....	E1582
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=400mL <600mL Frozen <=24h	E1578

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=400mL <600mL Frozen <=24h Aphr not automated	E1579
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=400mL <600mL Frozen >24h	E1580
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=400mL <600mL Frozen >24h Aphr not automated	E1581
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=600mL.....	E1583
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=600mL Aphr not automated	E1588
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=600mL Frozen <=24h	E1584
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=600mL Frozen <=24h Aphr not automated	E1585
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=600mL Frozen >24h	E1586
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated >=600mL Frozen >24h Aphr not automated	E1587
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated Aphr not automated	E1593
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated Frozen <=24h	E1589
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated Frozen <=24h Aphr not automated	E1590
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated Frozen >24h	E1591
APHERESIS PLASMA ACD-A/XX/<=-18C Irradiated Frozen >24h Aphr not automated	E1592
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf	E1522
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf <200 mL.....	E1529
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf <200 mL Aphr not automated	E1534
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf <200 mL Frozen <=24h	E1530
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf <200 mL Frozen <=24h Aphr not automated.....	E1531
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf <200 mL Frozen >24h.....	E1532
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf <200 mL Frozen >24h Aphr not automated	E1533
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=200 mL <400mL.....	E1535
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=200 mL <400mL Aphr not automated	E1540
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=200 mL <400mL Frozen <=24h	E1536
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=200 mL <400mL Frozen <=24h Aphr not automated	E1537
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=200 mL <400mL Frozen >24h.....	E1538
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=200 mL <400mL Frozen >24h Aphr not automated	E1539

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=400mL <600mL	E1541
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=400mL <600mL Aphr not automated	E1546
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=400mL <600mL Frozen <=24h.....	E1542
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=400mL <600mL Frozen <=24h Aphr not automated	E1543
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=400mL <600mL Frozen >24h	E1544
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=400mL <600mL Frozen >24h Aphr not automated	E1545
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=600mL	E1547
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=600mL Aphr not automated.....	E1552
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=600mL Frozen <=24h	E1548
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=600mL Frozen <=24h Aphr not automated.....	E1549
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=600mL Frozen >24h.....	E1550
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf >=600mL Frozen >24h Aphr not automated	E1551
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf Aphr not automated.....	E1557
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf Frozen <=24h	E1553
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf Frozen <=24h Aphr not automated	E1554
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf Frozen >24h.....	E1555
APHERESIS PLASMA ACD-A/XX/<=-18C Not for tx or mnf Frozen >24h Aphr not automated	E1556
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable.....	E1737
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable <200 mL	E1742
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable <200 mL Aphr not automated	E1745
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable <200 mL Frozen <=15h.....	E1743
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable <200 mL Frozen <=15h Aphr not automated	E1744
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=200 mL <400mL	E1746
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=200 mL <400mL Aphr not automated	E1749
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=200 mL <400mL Frozen <=15h.....	E1747
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=200 mL <400mL Frozen <=15h Aphr not automated	E1748
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=400mL <600mL	E1750

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=400mL <600mL Aphr not automated.....	E1753
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=400mL <600mL Frozen <=15h	E1751
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=400mL <600mL Frozen <=15h Aphr not automated	E1752
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=600mL.....	E1754
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=600mL Aphr not automated	E1757
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=600mL Frozen <=15h.....	E1755
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable >=600mL Frozen <=15h Aphr not automated	E1756
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable Aphr not automated	E1760
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable Frozen <=15h	E1758
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:injectable Frozen <=15h Aphr not automated	E1759
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable.....	E1761
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable <200 mL.....	E1766
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable <200 mL Aphr not automated	E1769
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable <200 mL Frozen <=15h.....	E1767
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable <200 mL Frozen <=15h Aphr not automated	E1768
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=200 mL <400mL	E1770
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=200 mL <400mL Aphr not automated	E1773
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=200 mL <400mL Frozen <=15h.....	E1771
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=200 mL <400mL Frozen <=15h Aphr not automated	E1772
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=400mL <600mL	E1774
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=400mL <600mL Aphr not automated	E1777
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=400mL <600mL Frozen <=15h.....	E1775
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=400mL <600mL Frozen <=15h Aphr not automated	E1776
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=600mL.....	E1778
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=600mL Aphr not automated	E1781
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=600mL Frozen <=15h.....	E1779
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable >=600mL Frozen <=15h Aphr not automated	E1780

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable Aphr not automated	E1784
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable Frozen <=15h	E1782
APHERESIS PLASMA ACD-A/XX/<=-20C For mnf:noninjectable Frozen <=15h Aphr not automated.....	E1783
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf	E1785
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf <200 mL.....	E1790
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf <200 mL Aphr not automated	E1793
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf <200 mL Frozen <=15h	E1791
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf <200 mL Frozen <=15h Aphr not automated.....	E1792
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=200 mL <400mL.....	E1794
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=200 mL <400mL Aphr not automated	E1797
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=200 mL <400mL Frozen <=15h.....	E1795
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=200 mL <400mL Frozen <=15h Aphr not automated	E1796
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=400mL <600mL	E1798
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=400mL <600mL Aphr not automated	E1801
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=400mL <600mL Frozen <=15h.....	E1799
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=400mL <600mL Frozen <=15h Aphr not automated	E1800
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=600mL	E1802
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=600mL Aphr not automated.....	E1805
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=600mL Frozen <=15h	E1803
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf >=600mL Frozen <=15h Aphr not automated.....	E1804
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf Aphr not automated.....	E1808
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf Frozen <=15h	E1806
APHERESIS PLASMA ACD-A/XX/<=-20C Not for tx or mnf Frozen <=15h Aphr not automated	E1807
APHERESIS PLASMA ACD-B/XX/<=-18C.....	E1413
APHERESIS PLASMA ACD-B/XX/<=-18C <200 mL	E1492
APHERESIS PLASMA ACD-B/XX/<=-18C <200 mL Aphr not automated	E1497
APHERESIS PLASMA ACD-B/XX/<=-18C <200 mL Frozen <=24h.....	E1493
APHERESIS PLASMA ACD-B/XX/<=-18C <200 mL Frozen <=24h Aphr not automated	E1494

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA ACD-B/XX/<=-18C <200 mL Frozen >24h	E1495
APHERESIS PLASMA ACD-B/XX/<=-18C <200 mL Frozen >24h Aphr not automated	E1496
APHERESIS PLASMA ACD-B/XX/<=-18C >=200 mL <400mL	E1498
APHERESIS PLASMA ACD-B/XX/<=-18C >=200 mL <400mL Aphr not automated	E1503
APHERESIS PLASMA ACD-B/XX/<=-18C >=200 mL <400mL Frozen <=24h	E1499
APHERESIS PLASMA ACD-B/XX/<=-18C >=200 mL <400mL Frozen <=24h Aphr not automated	E1500
APHERESIS PLASMA ACD-B/XX/<=-18C >=200 mL <400mL Frozen >24h	E1501
APHERESIS PLASMA ACD-B/XX/<=-18C >=200 mL <400mL Frozen >24h Aphr not automated	E1502
APHERESIS PLASMA ACD-B/XX/<=-18C >=400mL <600mL	E1504
APHERESIS PLASMA ACD-B/XX/<=-18C >=400mL <600mL Aphr not automated.....	E1509
APHERESIS PLASMA ACD-B/XX/<=-18C >=400mL <600mL Frozen <=24h	E1505
APHERESIS PLASMA ACD-B/XX/<=-18C >=400mL <600mL Frozen <=24h Aphr not automated	E1506
APHERESIS PLASMA ACD-B/XX/<=-18C >=400mL <600mL Frozen >24h	E1507
APHERESIS PLASMA ACD-B/XX/<=-18C >=400mL <600mL Frozen >24h Aphr not automated.....	E1508
APHERESIS PLASMA ACD-B/XX/<=-18C >=600mL.....	E1510
APHERESIS PLASMA ACD-B/XX/<=-18C >=600mL Aphr not automated	E1515
APHERESIS PLASMA ACD-B/XX/<=-18C >=600mL Frozen <=24h.....	E1511
APHERESIS PLASMA ACD-B/XX/<=-18C >=600mL Frozen <=24h Aphr not automated	E1512
APHERESIS PLASMA ACD-B/XX/<=-18C >=600mL Frozen >24h	E1513
APHERESIS PLASMA ACD-B/XX/<=-18C >=600mL Frozen >24h Aphr not automated	E1514
APHERESIS PLASMA ACD-B/XX/<=-18C Aphr not automated	E1520
APHERESIS PLASMA ACD-B/XX/<=-18C Frozen <=24h	E1516
APHERESIS PLASMA ACD-B/XX/<=-18C Frozen <=24h Aphr not automated	E1517
APHERESIS PLASMA ACD-B/XX/<=-18C Frozen >24h	E1518
APHERESIS PLASMA ACD-B/XX/<=-18C Frozen >24h Aphr not automated	E1519
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated.....	E1450
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated <200 mL	E1457
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated <200 mL Aphr not automated	E1462
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated <200 mL Frozen <=24h.....	E1458
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated <200 mL Frozen <=24h Aphr not automated	E1459

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated <200 mL Frozen >24h	E1460
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated <200 mL Frozen >24h Aphr not automated	E1461
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=200 mL <400mL	E1463
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=200 mL <400mL Aphr not automated	E1468
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=200 mL <400mL Frozen <=24h	E1464
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=200 mL <400mL Frozen <=24h Aphr not automated	E1465
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=200 mL <400mL Frozen >24h	E1466
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=200 mL <400mL Frozen >24h Aphr not automated	E1467
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=400mL <600mL	E1469
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=400mL <600mL Aphr not automated	E1474
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=400mL <600mL Frozen <=24h	E1470
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=400mL <600mL Frozen <=24h Aphr not automated	E1471
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=400mL <600mL Frozen >24h	E1472
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=400mL <600mL Frozen >24h Aphr not automated	E1473
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=600mL	E1475
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=600mL Aphr not automated	E1480
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=600mL Frozen <=24h	E1476
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=600mL Frozen <=24h Aphr not automated	E1477
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=600mL Frozen >24h	E1478
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated >=600mL Frozen >24h Aphr not automated	E1479
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated Aphr not automated	E1485
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated Frozen <=24h	E1481
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated Frozen <=24h Aphr not automated	E1482
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated Frozen >24h	E1483
APHERESIS PLASMA ACD-B/XX/<=-18C Irradiated Frozen >24h Aphr not automated	E1484
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf	E1414
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf <200 mL	E1421
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf <200 mL Aphr not automated	E1426

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf <200 mL Frozen <=24h	E1422
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf <200 mL Frozen <=24h Aphr not automated.....	E1423
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf <200 mL Frozen >24h.....	E1424
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf <200 mL Frozen >24h Aphr not automated	E1425
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=200 mL <400mL.....	E1427
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=200 mL <400mL Aphr not automated	E1432
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=200 mL <400mL Frozen <=24h.....	E1428
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=200 mL <400mL Frozen <=24h Aphr not	E1429
automated	
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=200 mL <400mL Frozen >24h.....	E1430
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=200 mL <400mL Frozen >24h Aphr not	E1431
automated	
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=400mL <600mL	E1433
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=400mL <600mL Aphr not automated	E1438
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=400mL <600mL Frozen <=24h.....	E1434
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=400mL <600mL Frozen <=24h Aphr not	E1435
automated	
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=400mL <600mL Frozen >24h	E1436
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=400mL <600mL Frozen >24h Aphr not	E1437
automated	
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=600mL	E1439
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=600mL Aphr not automated.....	E1444
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=600mL Frozen <=24h	E1440
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=600mL Frozen <=24h Aphr not automated.....	E1441
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=600mL Frozen >24h.....	E1442
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf >=600mL Frozen >24h Aphr not automated	E1443
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf Aphr not automated.....	E1449
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf Frozen <=24h	E1445
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf Frozen <=24h Aphr not automated	E1446
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf Frozen >24h.....	E1447
APHERESIS PLASMA ACD-B/XX/<=-18C Not for tx or mnf Frozen >24h Aphr not automated	E1448

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable.....	E1809
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable <200 mL	E1814
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable <200 mL Aphr not automated	E1817
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable <200 mL Frozen <=15h.....	E1815
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable <200 mL Frozen <=15h Aphr not	E1816
automated	
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=200 mL <400mL	E1818
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=200 mL <400mL Aphr not automated	E1821
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=200 mL <400mL Frozen <=15h.....	E1819
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=200 mL <400mL Frozen <=15h Aphr not	E1820
automated	
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=400mL <600mL	E1822
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=400mL <600mL Aphr not automated	E1825
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=400mL <600mL Frozen <=15h	E1823
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=400mL <600mL Frozen <=15h Aphr not	E1824
automated	
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=600mL.....	E1826
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=600mL Aphr not automated	E1829
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=600mL Frozen <=15h.....	E1827
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable >=600mL Frozen <=15h Aphr not	E1828
automated	
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable Aphr not automated	E1832
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable Frozen <=15h	E1830
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:injectable Frozen <=15h Aphr not automated	E1831
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable	E1833
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable <200 mL.....	E1838
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable <200 mL Aphr not automated	E1841
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable <200 mL Frozen <=15h	E1839
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable <200 mL Frozen <=15h Aphr not	E1840
automated	
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=200 mL <400mL	E1842
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=200 mL <400mL Aphr not automated	E1845

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=200 mL <400mL Frozen <=15h.....	E1843
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=200 mL <400mL Frozen <=15h Aphr not automated	E1844
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=400mL <600mL	E1846
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=400mL <600mL Aphr not automated	E1849
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=400mL <600mL Frozen <=15h.....	E1847
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=400mL <600mL Frozen <=15h Aphr not automated	E1848
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=600mL	E1850
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=600mL Aphr not automated	E1853
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=600mL Frozen <=15h	E1851
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable >=600mL Frozen <=15h Aphr not automated	E1852
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable Aphr not automated	E1856
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable Frozen <=15h	E1854
APHERESIS PLASMA ACD-B/XX/<=-20C For mnf:noninjectable Frozen <=15h Aphr not automated.....	E1855
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf	E1857
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf <200 mL.....	E1862
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf <200 mL Aphr not automated	E1865
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf <200 mL Frozen <=15h	E1863
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf <200 mL Frozen <=15h Aphr not automated.....	E1864
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=200 mL <400mL.....	E1866
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=200 mL <400mL Aphr not automated	E1869
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=200 mL <400mL Frozen <=15h.....	E1867
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=200 mL <400mL Frozen <=15h Aphr not automated	E1868
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=400mL <600mL	E1870
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=400mL <600mL Aphr not automated	E1873
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=400mL <600mL Frozen <=15h.....	E1871
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=400mL <600mL Frozen <=15h Aphr not automated	E1872
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=600mL	E1874

Product Description

Product Code

APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=600mL Aphr not automated.....	E1877
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=600mL Frozen <=15h	E1875
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf >=600mL Frozen <=15h Aphr not automated.....	E1876
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf Aphr not automated.....	E1880
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf Frozen <=15h	E1878
APHERESIS PLASMA ACD-B/XX/<=-20C Not for tx or mnf Frozen <=15h Aphr not automated.....	E1879
APHERESIS PLASMA NaCitrate/XX/<=-18C	E1629
APHERESIS PLASMA NaCitrate/XX/<=-18C <200 mL	E1708
APHERESIS PLASMA NaCitrate/XX/<=-18C <200 mL Aphr not automated	E1713
APHERESIS PLASMA NaCitrate/XX/<=-18C <200 mL Frozen <=24h	E1709
APHERESIS PLASMA NaCitrate/XX/<=-18C <200 mL Frozen <=24h Aphr not automated	E1710
APHERESIS PLASMA NaCitrate/XX/<=-18C <200 mL Frozen >24h	E1711
APHERESIS PLASMA NaCitrate/XX/<=-18C <200 mL Frozen >24h Aphr not automated	E1712
APHERESIS PLASMA NaCitrate/XX/<=-18C >=200 mL <400mL	E1714
APHERESIS PLASMA NaCitrate/XX/<=-18C >=200 mL <400mL Aphr not automated	E1719
APHERESIS PLASMA NaCitrate/XX/<=-18C >=200 mL <400mL Frozen <=24h	E1715
APHERESIS PLASMA NaCitrate/XX/<=-18C >=200 mL <400mL Frozen <=24h Aphr not automated	E1716
APHERESIS PLASMA NaCitrate/XX/<=-18C >=200 mL <400mL Frozen >24h	E1717
APHERESIS PLASMA NaCitrate/XX/<=-18C >=200 mL <400mL Frozen >24h Aphr not automated	E1718
APHERESIS PLASMA NaCitrate/XX/<=-18C >=400mL <600mL	E1720
APHERESIS PLASMA NaCitrate/XX/<=-18C >=400mL <600mL Aphr not automated	E1725
APHERESIS PLASMA NaCitrate/XX/<=-18C >=400mL <600mL Frozen <=24h	E1721
APHERESIS PLASMA NaCitrate/XX/<=-18C >=400mL <600mL Frozen <=24h Aphr not automated	E1722
APHERESIS PLASMA NaCitrate/XX/<=-18C >=400mL <600mL Frozen >24h	E1723
APHERESIS PLASMA NaCitrate/XX/<=-18C >=400mL <600mL Frozen >24h Aphr not automated	E1724
APHERESIS PLASMA NaCitrate/XX/<=-18C >=600mL	E1726
APHERESIS PLASMA NaCitrate/XX/<=-18C >=600mL Aphr not automated	E1731
APHERESIS PLASMA NaCitrate/XX/<=-18C >=600mL Frozen <=24h.....	E1727
APHERESIS PLASMA NaCitrate/XX/<=-18C >=600mL Frozen <=24h Aphr not automated	E1728

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA NaCitrate/XX<=-18C >=600mL Frozen >24h	E1729
APHERESIS PLASMA NaCitrate/XX<=-18C >=600mL Frozen >24h Aphr not automated	E1730
APHERESIS PLASMA NaCitrate/XX<=-18C Aphr not automated	E1736
APHERESIS PLASMA NaCitrate/XX<=-18C Frozen <=24h.....	E1732
APHERESIS PLASMA NaCitrate/XX<=-18C Frozen <=24h Aphr not automated	E1733
APHERESIS PLASMA NaCitrate/XX<=-18C Frozen >24h	E1734
APHERESIS PLASMA NaCitrate/XX<=-18C Frozen >24h Aphr not automated	E1735
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated	E1666
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated <200 mL	E1673
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated <200 mL Aphr not automated.....	E1678
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated <200 mL Frozen <=24h	E1674
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated <200 mL Frozen <=24h Aphr not automated	E1675
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated <200 mL Frozen >24h	E1676
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated <200 mL Frozen >24h Aphr not automated.....	E1677
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=200 mL <400mL	E1679
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=200 mL <400mL Aphr not automated.....	E1684
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=200 mL <400mL Frozen <=24h	E1680
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=200 mL <400mL Frozen <=24h Aphr not automated	E1681
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=200 mL <400mL Frozen >24h	E1682
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=200 mL <400mL Frozen >24h Aphr not automated	E1683
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=400mL <600mL	E1685
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=400mL <600mL Aphr not automated.....	E1690
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=400mL <600mL Frozen <=24h	E1686
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=400mL <600mL Frozen <=24h Aphr not automated	E1687
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=400mL <600mL Frozen >24h	E1688
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=400mL <600mL Frozen >24h Aphr not automated	E1689
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=600mL	E1691
APHERESIS PLASMA NaCitrate/XX<=-18C Irradiated >=600mL Aphr not automated	E1696

Product Description **Product Code**

APHERESIS PLASMA NaCitrate/XX <=-18C Irradiated >=600mL Frozen <=24h.....	E1692
APHERESIS PLASMA NaCitrate/XX <=-18C Irradiated >=600mL Frozen <=24h Aphr not automated	E1693
APHERESIS PLASMA NaCitrate/XX <=-18C Irradiated >=600mL Frozen >24h	E1694
APHERESIS PLASMA NaCitrate/XX <=-18C Irradiated >=600mL Frozen >24h Aphr not automated	E1695
APHERESIS PLASMA NaCitrate/XX <=-18C Irradiated Aphr not automated	E1701
APHERESIS PLASMA NaCitrate/XX <=-18C Irradiated Frozen <=24h.....	E1697
APHERESIS PLASMA NaCitrate/XX <=-18C Irradiated Frozen <=24h Aphr not automated	E1698
APHERESIS PLASMA NaCitrate/XX <=-18C Irradiated Frozen >24h	E1699
APHERESIS PLASMA NaCitrate/XX <=-18C Irradiated Frozen >24h Aphr not automated	E1700
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf.....	E1630
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf <200 mL.....	E1637
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf <200 mL Aphr not automated	E1642
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf <200 mL Frozen <=24h.....	E1638
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf <200 mL Frozen <=24h Aphr not	E1639
automated	
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf <200 mL Frozen >24h	E1640
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf <200 mL Frozen >24h Aphr not automated	E1641
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=200 mL <400mL	E1643
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=200 mL <400mL Aphr not automated	E1648
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=200 mL <400mL Frozen <=24h.....	E1644
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=200 mL <400mL Frozen <=24h Aphr	E1645
not automated	
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=200 mL <400mL Frozen >24h	E1646
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=200 mL <400mL Frozen >24h Aphr not	E1647
automated	
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=400mL <600mL	E1649
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=400mL <600mL Aphr not automated	E1654
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=400mL <600mL Frozen <=24h	E1650
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=400mL <600mL Frozen <=24h Aphr not.....	E1651
automated	
APHERESIS PLASMA NaCitrate/XX <=-18C Not for tx or mnf >=400mL <600mL Frozen >24h	E1652

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA NaCitrate/XX/<=-18C Not for tx or mnf >=400mL <600mL Frozen >24h Aphr not automated	E1653

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|>=600mL..... E1655

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|>=600mL|Aphr not automated E1660

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|>=600mL|Frozen <=24h E1656

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|>=600mL|Frozen <=24h|Aphr not automated E1657

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|>=600mL|Frozen >24h..... E1658

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|>=600mL|Frozen >24h|Aphr not automated
 E1659 |

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|Aphr not automated
 E1665 |

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|Frozen <=24h
 E1661 |

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|Frozen <=24h|Aphr not automated..... E1662

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|Frozen >24h..... E1663

APHERESIS PLASMA|NaCitrate/XX/<=-18C|Not for tx or mnf|Frozen >24h|Aphr not automated
 E1664 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable
 E1881 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|<200 mL
 E1886 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|<200 mL|Aphr not automated..... E1889

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|<200 mL|Frozen <=15h
 E1887 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|<200 mL|Frozen <=15h|Aphr not automated
 E1888 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=200 mL <400mL
 E1890 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=200 mL <400mL|Aphr not automated..... E1893

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=200 mL <400mL|Frozen <=15h
 E1891 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=200 mL <400mL|Frozen <=15h|Aphr not automated
 E1892 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=400mL <600mL
 E1894 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=400mL <600mL|Aphr not automated..... E1897

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=400mL <600mL|Frozen <=15h
 E1895 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=400mL <600mL|Frozen <=15h|Aphr not automated
 E1896 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=600mL
 E1898 |

APHERESIS PLASMA|NaCitrate/XX/<=-20C|For mnf:injectable|>=600mL|Aphr not automated
 E1901 |

Product Description

Product Code

APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:injectable >=600mL Frozen <=15h.....	E1899
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:injectable >=600mL Frozen <=15h Aphr not automated	E1900
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:injectable Aphr not automated	E1904
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:injectable Frozen <=15h.....	E1902
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:injectable Frozen <=15h Aphr not automated	E1903
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable.....	E1905
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable <200 mL	E1910
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable <200 mL Aphr not automated	E1913
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable <200 mL Frozen <=15h.....	E1911
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable <200 mL Frozen <=15h Aphr not automated	E1912
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=200 mL <400mL	E1914
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=200 mL <400mL Aphr not automated	E1917
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=200 mL <400mL Frozen <=15h	E1915
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=200 mL <400mL Frozen <=15h Aphr not automated	E1916
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=400mL <600mL	E1918
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=400mL <600mL Aphr not automated	E1921
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=400mL <600mL Frozen <=15h	E1919
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=400mL <600mL Frozen <=15h Aphr not automated	E1920
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=600mL	E1922
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=600mL Aphr not automated	E1925
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=600mL Frozen <=15h.....	E1923
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable >=600mL Frozen <=15h Aphr not automated	E1924
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable Aphr not automated	E1928
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable Frozen <=15h.....	E1926
APHERESIS PLASMA NaCitrate/XX<=-20C For mnf:noninjectable Frozen <=15h Aphr not automated	E1927
APHERESIS PLASMA NaCitrate/XX<=-20C Not for tx or mnf.....	E1929

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf <200 mL.....	E1934
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf <200 mL Aphr not automated	E1937
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf <200 mL Frozen <=15h.....	E1935
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf <200 mL Frozen <=15h Aphr not automated	E1936
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=200 mL <400mL	E1938
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=200 mL <400mL Aphr not automated	E1941
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=200 mL <400mL Frozen <=15h.....	E1939
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=200 mL <400mL Frozen <=15h Aphr not automated	E1940
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=400mL <600mL	E1942
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=400mL <600mL Aphr not automated	E1945
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=400mL <600mL Frozen <=15h	E1943
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=400mL <600mL Frozen <=15h Aphr not automated	E1944
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=600mL.....	E1946
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=600mL Aphr not automated	E1949
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=600mL Frozen <=15h	E1947
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf >=600mL Frozen <=15h Aphr not automated	E1948
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf Aphr not automated	E1952
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf Frozen <=15h	E1950
APHERESIS PLASMA NaCitrate/XX/<=-20C Not for tx or mnf Frozen <=15h Aphr not automated.....	E1951
APHERESIS PLATELETS ACD-A/XX/<37C For mnf:injectable.....	E2934
APHERESIS PLATELETS ACD-A/XX/<37C For mnf:noninjectable.....	E2935
APHERESIS PLATELETS ACD-A/XX/<37C Not for tx or mnf	E2936
APHERESIS PLATELETS ACD-A/XX/20-24C	E2940
APHERESIS PLATELETS ACD-A/XX/20-24C 1st container.....	E3102
APHERESIS PLATELETS ACD-A/XX/20-24C 1st container:not auto	E3106
APHERESIS PLATELETS ACD-A/XX/20-24C 2nd container.....	E3103
APHERESIS PLATELETS ACD-A/XX/20-24C 2nd container:not auto	E3107

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-A/XX/20-24C 3rd container	E3104
APHERESIS PLATELETS ACD-A/XX/20-24C 4th container	E3105
APHERESIS PLATELETS ACD-A/XX/20-24C Aphr not automated.....	E3101
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:injectable	E2941
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:injectable 1st container.....	E2943
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:injectable 1st container:not auto	E2947
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:injectable 2nd container.....	E2944
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:injectable 2nd container:not auto	E2948
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:injectable 3rd container	E2945
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:injectable 4th container	E2946
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:injectable Aphr not automated.....	E2942
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable	E2949
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable 1st container	E2959
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable 1st container:not auto	E2963
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable 2nd container	E2960
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable 2nd container:not auto.....	E2964
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable 3rd container.....	E2961
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable 4th container.....	E2962
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable Aphr not automated	E2958
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable Open	E2950
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable Open 1st container	E2952
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable Open 1st container:not auto.....	E2956
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable Open 2nd container	E2953
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable Open 2nd container:not auto.....	E2957
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable Open 3rd container.....	E2954
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable Open 4th container	E2955
APHERESIS PLATELETS ACD-A/XX/20-24C For mnf:noninjectable Open Aphr not automated	E2951
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated	E3045
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated 1st container.....	E3071
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated 1st container:not auto	E3075

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated 2nd container.....	E3072
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated 2nd container:not auto	E3076
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated 3rd container	E3073
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated 4th container	E3074
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated Aphr not automated.....	E3070
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated Plasma reduced	E3062
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated Plasma reduced 1st container.....	E3064
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated Plasma reduced 1st container:not auto	E3068
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated Plasma reduced 2nd container	E3065
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated Plasma reduced 2nd container:not auto	E3069
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated Plasma reduced 3rd container	E3066
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated Plasma reduced 4th container.....	E3067
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated Plasma reduced Aphr not automated.....	E3063
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<1log6.....	E3929
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<1log6 Plasma reduced	E3931
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 120 log9 plts	E3981
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 180 log9 plts	E3982
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 240 log9 plts	E3997
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 300 log9 plts	E3998
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 360 log9 plts	E3999
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 420 log9 plts	E4000
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 480 log9 plts	E4001
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Plasma reduced Approx 120 log9	E3976
plts	
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Plasma reduced Approx 180 log9	E3975
plts	
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Plasma reduced Approx 240 log9	E3974
plts	
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6.....	E3046
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 1st container	E3056
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 1st container:not auto	E3060

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 2nd container	E3057
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 2nd container:not auto	E3061
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 3rd container	E3058
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 4th container	E3059
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 Aphr not automated	E3055
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced	E3047
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 1st container	E3049
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 1st container:not auto	E3053
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 2nd container	E3050
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 2nd container:not auto	E3054
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 3rd container	E3051
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 4th container	E3052
APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced Aphr not automated	E3048
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf	E2965
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf 1st container	E2975
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf 1st container:not auto	E2979
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf 2nd container	E2976
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf 2nd container:not auto	E2980
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf 3rd container	E2977
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf 4th container	E2978
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf Aphr not automated	E2974
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf Open	E2966
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf Open 1st container	E2968
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf Open 1st container:not auto	E2972
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf Open 2nd container	E2969
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf Open 2nd container:not auto	E2973
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf Open 3rd container	E2970

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf Open 4th container	E2971
APHERESIS PLATELETS ACD-A/XX/20-24C Not for tx or mnf Open Aphr not automated	E2967
APHERESIS PLATELETS ACD-A/XX/20-24C Open	E2981
APHERESIS PLATELETS ACD-A/XX/20-24C Open 1st container.....	E3039
APHERESIS PLATELETS ACD-A/XX/20-24C Open 1st container:not auto	E3043
APHERESIS PLATELETS ACD-A/XX/20-24C Open 2nd container	E3040
APHERESIS PLATELETS ACD-A/XX/20-24C Open 2nd container:not auto	E3044
APHERESIS PLATELETS ACD-A/XX/20-24C Open 3rd container	E3041
APHERESIS PLATELETS ACD-A/XX/20-24C Open 4th container.....	E3042
APHERESIS PLATELETS ACD-A/XX/20-24C Open Aphr not automated.....	E3038
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated	E2982
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated 1st container.....	E3008
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated 1st container:not auto	E3012
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated 2nd container	E3009
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated 2nd container:not auto	E3013
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated 3rd container	E3010
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated 4th container.....	E3011
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated Aphr not automated.....	E3007
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated Plasma reduced	E2999
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated Plasma reduced 1st container	E3001
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated Plasma reduced 1st container:not auto.....	E3005
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated Plasma reduced 2nd container	E3002
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated Plasma reduced 2nd container:not auto.....	E3006
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated Plasma reduced 3rd container.....	E3003
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated Plasma reduced 4th container	E3004
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated Plasma reduced Aphr not automated	E3000
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6	E2983
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 1st container	E2993
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 1st container:not auto	E2997

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 2nd container	E2994
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 2nd container:not auto	E2998
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 3rd container	E2995
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 4th container	E2996
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 Aphr not automated	E2992
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced	E2984
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 1st container	E2986
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 1st container:not auto	E2990
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 2nd container	E2987
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 2nd container:not auto	E2991
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 3rd container	E2988
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 4th container	E2989
APHERESIS PLATELETS ACD-A/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced Aphr not automated	E2985
APHERESIS PLATELETS ACD-A/XX/20-24C Open Plasma reduced	E3030
APHERESIS PLATELETS ACD-A/XX/20-24C Open Plasma reduced 1st container	E3032
APHERESIS PLATELETS ACD-A/XX/20-24C Open Plasma reduced 1st container:not auto	E3036
APHERESIS PLATELETS ACD-A/XX/20-24C Open Plasma reduced 2nd container	E3033
APHERESIS PLATELETS ACD-A/XX/20-24C Open Plasma reduced 2nd container:not auto	E3037
APHERESIS PLATELETS ACD-A/XX/20-24C Open Plasma reduced 3rd container	E3034
APHERESIS PLATELETS ACD-A/XX/20-24C Open Plasma reduced 4th container	E3035
APHERESIS PLATELETS ACD-A/XX/20-24C Open Plasma reduced Aphr not automated	E3031
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6	E3014
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 1st container	E3024
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 1st container:not auto	E3028
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 2nd container	E3025
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 2nd container:not auto	E3029
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 3rd container	E3026

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 4th container	E3027
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 Aphr not automated	E3023
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 Plasma reduced	E3015
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 Plasma reduced 1st container.....	E3017
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 Plasma reduced 1st container:not auto	E3021
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 Plasma reduced 2nd container.....	E3018
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 Plasma reduced 2nd container:not auto	E3022
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 Plasma reduced 3rd container	E3019
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 Plasma reduced 4th container	E3020
APHERESIS PLATELETS ACD-A/XX/20-24C Open ResLeu:<5log6 Plasma reduced Aphr not automated.....	E3016
APHERESIS PLATELETS ACD-A/XX/20-24C Plasma reduced	E3093
APHERESIS PLATELETS ACD-A/XX/20-24C Plasma reduced 1st container	E3095
APHERESIS PLATELETS ACD-A/XX/20-24C Plasma reduced 1st container:not auto	E3099
APHERESIS PLATELETS ACD-A/XX/20-24C Plasma reduced 2nd container	E3096
APHERESIS PLATELETS ACD-A/XX/20-24C Plasma reduced 2nd container:not auto	E3100
APHERESIS PLATELETS ACD-A/XX/20-24C Plasma reduced 3rd container	E3097
APHERESIS PLATELETS ACD-A/XX/20-24C Plasma reduced 4th container	E3098
APHERESIS PLATELETS ACD-A/XX/20-24C Plasma reduced Aphr not automated	E3094
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<1log6.....	E3928
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<1log6 Plasma reduced	E3930
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<2log5 Approx 120 log9 plts	E4002
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<2log5 Approx 180 log9 plts	E4003
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<2log5 Approx 240 log9 plts	E3843
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<2log5 Approx 300 log9 plts	E3980
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<2log5 Approx 360 log9 plts	E3979
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<2log5 Approx 420 log9 plts	E3978
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<2log5 Approx 480 log9 plts	E3977
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6.....	E3077

Product Description

Product Code

APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 1st container	E3087
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 1st container:not auto	E3091
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 2nd container	E3088
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 2nd container:not auto	E3092
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 3rd container	E3089
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 4th container	E3090
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 Aphr not automated	E3086
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 Plasma reduced	E3078
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 Plasma reduced 1st container	E3080
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 Plasma reduced 1st container:not auto	E3084
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 Plasma reduced 2nd container	E3081
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 Plasma reduced 2nd container:not auto	E3085
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 Plasma reduced 3rd container	E3082
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 Plasma reduced 4th container	E3083
APHERESIS PLATELETS ACD-A/XX/20-24C ResLeu:<5log6 Plasma reduced Aphr not automated	E3079
APHERESIS PLATELETS ACD-A/XX/refg	E2926
APHERESIS PLATELETS ACD-A/XX/refg For mnf:injectable.....	E2927
APHERESIS PLATELETS ACD-A/XX/refg For mnf:noninjectable.....	E2928
APHERESIS PLATELETS ACD-A/XX/refg Not for tx or mnf	E2929
APHERESIS PLATELETS ACD-B/XX/<37C For mnf:injectable.....	E2937
APHERESIS PLATELETS ACD-B/XX/<37C For mnf:noninjectable.....	E2938
APHERESIS PLATELETS ACD-B/XX/<37C Not for tx or mnf	E2939
APHERESIS PLATELETS ACD-B/XX/20-24C	E3108
APHERESIS PLATELETS ACD-B/XX/20-24C 1st container.....	E3270
APHERESIS PLATELETS ACD-B/XX/20-24C 1st container:not auto	E3274
APHERESIS PLATELETS ACD-B/XX/20-24C 2nd container.....	E3271
APHERESIS PLATELETS ACD-B/XX/20-24C 2nd container:not auto	E3275
APHERESIS PLATELETS ACD-B/XX/20-24C 3rd container	E3272
APHERESIS PLATELETS ACD-B/XX/20-24C 4th container	E3273

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-B/XX/20-24C Aphr not automated.....	E3269
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:injectable	E3109
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:injectable 1st container.....	E3111
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:injectable 1st container:not auto	E3115
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:injectable 2nd container	E3112
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:injectable 2nd container:not auto	E3116
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:injectable 3rd container	E3113
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:injectable 4th container	E3114
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:injectable Aphr not automated.....	E3110
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable	E3117
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable 1st container	E3127
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable 1st container:not auto	E3131
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable 2nd container	E3128
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable 2nd container:not auto.....	E3132
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable 3rd container.....	E3129
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable 4th container	E3130
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable Aphr not automated.....	E3126
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable Open	E3118
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable Open 1st container	E3120
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable Open 1st container:not auto.....	E3124
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable Open 2nd container	E3121
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable Open 2nd container:not auto.....	E3125
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable Open 3rd container.....	E3122
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable Open 4th container	E3123
APHERESIS PLATELETS ACD-B/XX/20-24C For mnf:noninjectable Open Aphr not automated	E3119
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated	E3213
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated 1st container.....	E3239
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated 1st container:not auto	E3243
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated 2nd container.....	E3240
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated 2nd container:not auto	E3244

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated 3rd container	E3241
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated 4th container	E3242
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated Aphr not automated.....	E3238
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated Plasma reduced	E3230
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated Plasma reduced 1st container.....	E3232
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated Plasma reduced 1st container:not auto	E3236
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated Plasma reduced 2nd container.....	E3233
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated Plasma reduced 2nd container:not auto	E3237
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated Plasma reduced 3rd container	E3234
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated Plasma reduced 4th container.....	E3235
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated Plasma reduced Aphr not automated.....	E3231
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6.....	E3214
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 1st container	E3224
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 1st container:not auto	E3228
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 2nd container	E3225
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 2nd container:not auto	E3229
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 3rd container	E3226
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 4th container	E3227
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 Aphr not automated	E3223
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced	E3215
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 1st container	E3217
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 1st container:not auto	E3221
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 2nd container	E3218
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 2nd container:not auto	E3222
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 3rd container	E3219
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced 4th container	E3220
APHERESIS PLATELETS ACD-B/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced Aphr not automated	E3216

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf	E3133
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf 1st container	E3143
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf 1st container:not auto.....	E3147
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf 2nd container	E3144
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf 2nd container:not auto.....	E3148
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf 3rd container.....	E3145
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf 4th container.....	E3146
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf Aphr not automated	E3142
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf Open.....	E3134
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf Open 1st container	E3136
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf Open 1st container:not auto.....	E3140
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf Open 2nd container	E3137
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf Open 2nd container:not auto.....	E3141
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf Open 3rd container	E3138
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf Open 4th container	E3139
APHERESIS PLATELETS ACD-B/XX/20-24C Not for tx or mnf Open Aphr not automated	E3135
APHERESIS PLATELETS ACD-B/XX/20-24C Open	E3149
APHERESIS PLATELETS ACD-B/XX/20-24C Open 1st container.....	E3207
APHERESIS PLATELETS ACD-B/XX/20-24C Open 1st container:not auto	E3211
APHERESIS PLATELETS ACD-B/XX/20-24C Open 2nd container	E3208
APHERESIS PLATELETS ACD-B/XX/20-24C Open 2nd container:not auto	E3212
APHERESIS PLATELETS ACD-B/XX/20-24C Open 3rd container	E3209
APHERESIS PLATELETS ACD-B/XX/20-24C Open 4th container.....	E3210
APHERESIS PLATELETS ACD-B/XX/20-24C Open Aphr not automated	E3206
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated	E3150
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated 1st container.....	E3176
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated 1st container:not auto	E3180
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated 2nd container	E3177
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated 2nd container:not auto	E3181
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated 3rd container	E3178

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated 4th container.....	E3179
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated Aphr not automated	E3175
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated Plasma reduced	E3167
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated Plasma reduced 1st container	E3169
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated Plasma reduced 1st container:not auto.....	E3173
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated Plasma reduced 2nd container	E3170
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated Plasma reduced 2nd container:not auto.....	E3174
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated Plasma reduced 3rd container.....	E3171
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated Plasma reduced 4th container	E3172
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated Plasma reduced Aphr not automated	E3168
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6	E3151
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 1st container	E3161
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 1st container:not auto	E3165
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 2nd container	E3162
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 2nd container:not auto	E3166
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 3rd container	E3163
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 4th container	E3164
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Aphr not automated	E3160
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced	E3152
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 1st	E3154
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 1st container:not auto	E3158
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 2nd	E3155
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 2nd container:not auto	E3159
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 3rd	E3156
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced 4th	E3157
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced Aphr not	E3153
APHERESIS PLATELETS ACD-B/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced Aphr not automated	

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS ACD-B/XX/20-24C Open Plasma reduced	E3198
APHERESIS PLATELETS ACD-B/XX/20-24C Open Plasma reduced 1st container	E3200
APHERESIS PLATELETS ACD-B/XX/20-24C Open Plasma reduced 1st container:not auto.....	E3204
APHERESIS PLATELETS ACD-B/XX/20-24C Open Plasma reduced 2nd container	E3201
APHERESIS PLATELETS ACD-B/XX/20-24C Open Plasma reduced 2nd container:not auto.....	E3205
APHERESIS PLATELETS ACD-B/XX/20-24C Open Plasma reduced 3rd container.....	E3202
APHERESIS PLATELETS ACD-B/XX/20-24C Open Plasma reduced 4th container	E3203
APHERESIS PLATELETS ACD-B/XX/20-24C Open Plasma reduced Aphr not automated	E3199
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6	E3182
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 1st container	E3192
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 1st container:not auto	E3196
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 2nd container	E3193
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 2nd container:not auto	E3197
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 3rd container	E3194
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 4th container	E3195
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 Aphr not automated	E3191
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 Plasma reduced	E3183
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 Plasma reduced 1st container.....	E3185
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 Plasma reduced 1st container:not auto	E3189
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 Plasma reduced 2nd container.....	E3186
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 Plasma reduced 2nd container:not auto	E3190
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 Plasma reduced 3rd container	E3187
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 Plasma reduced 4th container	E3188
APHERESIS PLATELETS ACD-B/XX/20-24C Open ResLeu:<5log6 Plasma reduced Aphr not automated.....	E3184
APHERESIS PLATELETS ACD-B/XX/20-24C Plasma reduced	E3261
APHERESIS PLATELETS ACD-B/XX/20-24C Plasma reduced 1st container.....	E3263
APHERESIS PLATELETS ACD-B/XX/20-24C Plasma reduced 1st container:not auto	E3267
APHERESIS PLATELETS ACD-B/XX/20-24C Plasma reduced 2nd container	E3264

Product Description

Product Code

APHERESIS PLATELETS ACD-B/XX/20-24C Plasma reduced 2nd container:not auto	E3268
APHERESIS PLATELETS ACD-B/XX/20-24C Plasma reduced 3rd container	E3265
APHERESIS PLATELETS ACD-B/XX/20-24C Plasma reduced 4th container.....	E3266
APHERESIS PLATELETS ACD-B/XX/20-24C Plasma reduced Aphr not automated.....	E3262
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6.....	E3245
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 1st container	E3255
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 1st container:not auto	E3259
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 2nd container	E3256
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 2nd container:not auto	E3260
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 3rd container	E3257
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 4th container	E3258
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 Aphr not automated	E3254
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 Plasma reduced	E3246
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 Plasma reduced 1st container	E3248
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 Plasma reduced 1st container:not auto	E3252
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 Plasma reduced 2nd container	E3249
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 Plasma reduced 2nd container:not auto	E3253
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 Plasma reduced 3rd container	E3250
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 Plasma reduced 4th container	E3251
APHERESIS PLATELETS ACD-B/XX/20-24C ResLeu:<5log6 Plasma reduced Aphr not automated	E3247
APHERESIS PLATELETS ACD-B/XX/refg	E2922
APHERESIS PLATELETS ACD-B/XX/refg For mnf:injectable.....	E2923
APHERESIS PLATELETS ACD-B/XX/refg For mnf:noninjectable.....	E2924
APHERESIS PLATELETS ACD-B/XX/refg Not for tx or mnf.....	E2925
APHERESIS PLATELETS NaCitrate/XX/refg	E2930
APHERESIS PLATELETS NaCitrate/XX/refg For mnf:injectable	E2931
APHERESIS PLATELETS NaCitrate/XX/refg For mnf:noninjectable	E2932
APHERESIS PLATELETS NaCitrate/XX/refg Not for tx or mnf.....	E2933
APHERESIS PLATELETS NS/XX/<37C For mnf:injectable.....	E3444

<u>Product Description</u>	<u>Product Code</u>
APHERESIS PLATELETS NS/XX/<37C For mnf:noninjectable.....	E3445
APHERESIS PLATELETS NS/XX/<37C Not for tx or mnf.....	E3446
APHERESIS PLATELETS NS/XX/20-24C	E3822
APHERESIS PLATELETS NS/XX/20-24C Irradiated	E3834
APHERESIS PLATELETS NS/XX/20-24C Irradiated ResLeu:<5log6.....	E3836
APHERESIS PLATELETS NS/XX/20-24C ResLeu:<5log6.....	E3835
APHERESIS RED BLOOD CELLS AS3/XX/refg	E0605
APHERESIS RED BLOOD CELLS AS3/XX/refg 1st container	E0693
APHERESIS RED BLOOD CELLS AS3/XX/refg 2nd container	E0694
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:injectable	E0606
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:injectable 1st container	E0610
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:injectable 2nd container	E0611
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:injectable Open.....	E0607
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:injectable Open 1st container	E0608
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:injectable Open 2nd container	E0609
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:noninjectable.....	E0612
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:noninjectable 1st container	E0616
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:noninjectable 2nd container	E0617
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:noninjectable Open	E0613
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:noninjectable Open 1st container	E0614
APHERESIS RED BLOOD CELLS AS3/XX/refg For mnf:noninjectable Open 2nd container	E0615
APHERESIS RED BLOOD CELLS AS3/XX/refg Irradiated	E0660
APHERESIS RED BLOOD CELLS AS3/XX/refg Irradiated 1st container	E0676
APHERESIS RED BLOOD CELLS AS3/XX/refg Irradiated 2nd container	E0677
APHERESIS RED BLOOD CELLS AS3/XX/refg Irradiated ResLeu:<5log6	E0661
APHERESIS RED BLOOD CELLS AS3/XX/refg Irradiated ResLeu:<5log6 1st container.....	E0668
APHERESIS RED BLOOD CELLS AS3/XX/refg Irradiated ResLeu:<5log6 2nd container.....	E0669
APHERESIS RED BLOOD CELLS AS3/XX/refg Irradiated ResLeu:<5log6 Supernat rem	E0662
APHERESIS RED BLOOD CELLS AS3/XX/refg Irradiated ResLeu:<5log6 Supernat rem/Plasma added	E0665

Product Description

Product Code

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|ResLeu:<5log6|Supernat rem/Plasma E0666
added|1st container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|ResLeu:<5log6|Supernat rem/Plasma E0667
added|2nd container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|ResLeu:<5log6|Supernat rem|1st container E0663

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|ResLeu:<5log6|Supernat rem|2nd container E0664

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|Supernat rem E0670

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|Supernat rem/Plasma added..... E0673

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|Supernat rem/Plasma added|1st container E0674

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|Supernat rem/Plasma added|2nd container E0675

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|Supernat rem|1st container..... E0671

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Irradiated|Supernat rem|2nd container..... E0672

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Not for tx or mnf..... E0618

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Not for tx or mnf|1st container E0622

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Not for tx or mnf|2nd container E0623

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Not for tx or mnf|Open E0619

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Not for tx or mnf|Open|1st container E0620

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Not for tx or mnf|Open|2nd container..... E0621

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open..... E0624

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|1st container E0658

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|2nd container E0659

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated..... E0625

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|1st container E0641

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|2nd container E0642

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|ResLeu:<5log6 E0626

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|ResLeu:<5log6|1st container E0633

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|ResLeu:<5log6|2nd container E0634

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|ResLeu:<5log6|Supernat rem E0627

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|ResLeu:<5log6|Supernat rem/Plasma E0630
added

<u>Product Description</u>	<u>Product Code</u>
-----------------------------------	----------------------------

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|ResLeu:<5log6|Supernat rem/Plasma E0631
added|1st container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|ResLeu:<5log6|Supernat rem/Plasma E0632
added|2nd container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|ResLeu:<5log6|Supernat rem|1st E0628
container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|ResLeu:<5log6|Supernat rem|2nd E0629
container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|Supernat rem E0635

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|Supernat rem/Plasma added..... E0638

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|Supernat rem/Plasma added|1st E0639
container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|Supernat rem/Plasma added|2nd E0640
container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|Supernat rem|1st container E0636

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Irradiated|Supernat rem|2nd container E0637

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|ResLeu:<5log6 E0643

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|ResLeu:<5log6|1st container E0650

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|ResLeu:<5log6|2nd container E0651

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|ResLeu:<5log6|Supernat rem E0644

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|ResLeu:<5log6|Supernat rem/Plasma added E0647

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|ResLeu:<5log6|Supernat rem/Plasma added|1st E0648
container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|ResLeu:<5log6|Supernat rem/Plasma added|2nd E0649
container

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|ResLeu:<5log6|Supernat rem|1st container E0645

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|ResLeu:<5log6|Supernat rem|2nd container E0646

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Supernat rem E0652

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Supernat rem/Plasma added..... E0655

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Supernat rem/Plasma added|1st container E0656

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Supernat rem/Plasma added|2nd container E0657

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Supernat rem|1st container..... E0653

APHERESIS RED BLOOD CELLS|AS3/XX/refg|Open|Supernat rem|2nd container..... E0654

APHERESIS RED BLOOD CELLS|AS3/XX/refg|ResLeu:<5log6 E0678

APHERESIS RED BLOOD CELLS|AS3/XX/refg|ResLeu:<5log6|1st container..... E0685

Product Description

Product Code

APHERESIS RED BLOOD CELLS AS3/XX/refg ResLeu:<5log6 2nd container	E0686
APHERESIS RED BLOOD CELLS AS3/XX/refg ResLeu:<5log6 Supernat rem	E0679
APHERESIS RED BLOOD CELLS AS3/XX/refg ResLeu:<5log6 Supernat rem/Plasma added	E0682
APHERESIS RED BLOOD CELLS AS3/XX/refg ResLeu:<5log6 Supernat rem/Plasma added 1st container	E0683
APHERESIS RED BLOOD CELLS AS3/XX/refg ResLeu:<5log6 Supernat rem/Plasma added 2nd container	E0684
APHERESIS RED BLOOD CELLS AS3/XX/refg ResLeu:<5log6 Supernat rem 1st container	E0680
APHERESIS RED BLOOD CELLS AS3/XX/refg ResLeu:<5log6 Supernat rem 2nd container	E0681
APHERESIS RED BLOOD CELLS AS3/XX/refg Supernat rem	E0687
APHERESIS RED BLOOD CELLS AS3/XX/refg Supernat rem/Plasma added.....	E0690
APHERESIS RED BLOOD CELLS AS3/XX/refg Supernat rem/Plasma added 1st container	E0691
APHERESIS RED BLOOD CELLS AS3/XX/refg Supernat rem/Plasma added 2nd container	E0692
APHERESIS RED BLOOD CELLS AS3/XX/refg Supernat rem 1st container.....	E0688
APHERESIS RED BLOOD CELLS AS3/XX/refg Supernat rem 2nd container.....	E0689
APHERESIS RED BLOOD CELLS SAGM/XX/refg Irradiated	E3839
CRYOPRECIPITATE None/450mL/<=-18C	E3571
CRYOPRECIPITATE None/450mL/<=-18C Irradiated	E3572
CRYOPRECIPITATE None/500mL/<=-18C	E3573
CRYOPRECIPITATE None/500mL/<=-18C Irradiated	E3574
CRYOPRECIPITATE NS/450mL/<-30C ResLeu:<5log6.....	E4006
Deglycerolized RED BLOOD CELLS None/250mL/refg Not for tx or mnf Open	E0543
Deglycerolized RED BLOOD CELLS None/250mL/refg Open.....	E0544
Deglycerolized RED BLOOD CELLS None/250mL/refg Open Albumin added.....	E0548
Deglycerolized RED BLOOD CELLS None/250mL/refg Open Irradiated.....	E0545
Deglycerolized RED BLOOD CELLS None/250mL/refg Open Irradiated Albumin added.....	E0546
Deglycerolized RED BLOOD CELLS None/250mL/refg Open Irradiated Plasma added	E0547
Deglycerolized RED BLOOD CELLS None/250mL/refg Open Plasma added	E0549
Deglycerolized RED BLOOD CELLS None/450mL/refg For mnf:injectable Open	E0525
Deglycerolized RED BLOOD CELLS None/450mL/refg For mnf:noninjectable Open	E0526
Deglycerolized RED BLOOD CELLS None/450mL/refg Not for tx or mnf Open	E0527

<u>Product Description</u>	<u>Product Code</u>
Deglycerolized RED BLOOD CELLS None/450mL/refg Open	E0528
Deglycerolized RED BLOOD CELLS None/450mL/refg Open Albumin added	E0532
Deglycerolized RED BLOOD CELLS None/450mL/refg Open Irradiated	E0529
Deglycerolized RED BLOOD CELLS None/450mL/refg Open Irradiated Albumin added	E0530
Deglycerolized RED BLOOD CELLS None/450mL/refg Open Irradiated Plasma added	E0531
Deglycerolized RED BLOOD CELLS None/450mL/refg Open Plasma added	E0533
Deglycerolized RED BLOOD CELLS None/450mL/rt ResLeu:<1log6 Supernat rem/Plasma added From 2 donors	E3942
Deglycerolized RED BLOOD CELLS None/450mL/rt ResLeu:<1log6 Supernat rem Quar:>=6m/retested	E3993
Deglycerolized RED BLOOD CELLS None/500mL/refg For mnf:injectable Open	E0534
Deglycerolized RED BLOOD CELLS None/500mL/refg For mnf:noninjectable Open	E0535
Deglycerolized RED BLOOD CELLS None/500mL/refg Not for tx or mnf Open	E0536
Deglycerolized RED BLOOD CELLS None/500mL/refg Open	E0537
Deglycerolized RED BLOOD CELLS None/500mL/refg Open Albumin added	E0541
Deglycerolized RED BLOOD CELLS None/500mL/refg Open Irradiated	E0538
Deglycerolized RED BLOOD CELLS None/500mL/refg Open Irradiated Albumin added	E0539
Deglycerolized RED BLOOD CELLS None/500mL/refg Open Irradiated Plasma added	E0540
Deglycerolized RED BLOOD CELLS None/500mL/refg Open Plasma added	E0542
Deglycerolized Rejuvenated RED BLOOD CELLS None/250mL/refg Not for tx or mnf Open	E0564
Deglycerolized Rejuvenated RED BLOOD CELLS None/250mL/refg Open	E0565
Deglycerolized Rejuvenated RED BLOOD CELLS None/250mL/refg Open Albumin added	E0569
Deglycerolized Rejuvenated RED BLOOD CELLS None/250mL/refg Open Irradiated	E0566
Deglycerolized Rejuvenated RED BLOOD CELLS None/250mL/refg Open Irradiated Albumin added	E0567
Deglycerolized Rejuvenated RED BLOOD CELLS None/250mL/refg Open Irradiated Plasma added	E0568
Deglycerolized Rejuvenated RED BLOOD CELLS None/250mL/refg Open Plasma added	E0570
Deglycerolized Rejuvenated RED BLOOD CELLS None/450mL/refg Not for tx or mnf Open	E0550
Deglycerolized Rejuvenated RED BLOOD CELLS None/450mL/refg Open	E0551
Deglycerolized Rejuvenated RED BLOOD CELLS None/450mL/refg Open Albumin added	E0555
Deglycerolized Rejuvenated RED BLOOD CELLS None/450mL/refg Open Irradiated	E0552
Deglycerolized Rejuvenated RED BLOOD CELLS None/450mL/refg Open Irradiated Albumin added	E0553

<u>Product Description</u>	<u>Product Code</u>
Deglycerolized Rejuvenated RED BLOOD CELLS None/450mL/refg Open Irradiated Plasma added	E0554
Deglycerolized Rejuvenated RED BLOOD CELLS None/450mL/refg Open Plasma added	E0556
Deglycerolized Rejuvenated RED BLOOD CELLS None/500mL/refg Not for tx or mnf Open	E0557
Deglycerolized Rejuvenated RED BLOOD CELLS None/500mL/refg Open.....	E0558
Deglycerolized Rejuvenated RED BLOOD CELLS None/500mL/refg Open Albumin added	E0562
Deglycerolized Rejuvenated RED BLOOD CELLS None/500mL/refg Open Irradiated.....	E0559
Deglycerolized Rejuvenated RED BLOOD CELLS None/500mL/refg Open Irradiated Albumin added	E0560
Deglycerolized Rejuvenated RED BLOOD CELLS None/500mL/refg Open Irradiated Plasma added	E0561
Deglycerolized Rejuvenated RED BLOOD CELLS None/500mL/refg Open Plasma added	E0563
FRESH FROZEN PLASMA CP2D/XX/<=-18C	E0713
FRESH FROZEN PLASMA CP2D/XX/<=-18C Irradiated	E0716
FRESH FROZEN PLASMA CP2D/XX/<=-18C Not for tx or mnf	E0714
FRESH FROZEN PLASMA CP2D/XX/<-65C.....	E0743
FRESH FROZEN PLASMA CP2D/XX/<-65C Irradiated.....	E0746
FRESH FROZEN PLASMA CP2D/XX/<-65C Not for tx or mnf	E0744
FRESH FROZEN PLASMA CPD/450mL/<=-18C For mnf:injectable Frozen <=24h.....	E3872
FRESH FROZEN PLASMA CPD/450mL/<=-18C For mnf:injectable Frozen <=6h	E3857
FRESH FROZEN PLASMA CPD/450mL/<=-18C For mnf:noninjectable Frozen <=6h	E3860
FRESH FROZEN PLASMA CPD/450mL/<=-18C Frozen <=6h	E3854
FRESH FROZEN PLASMA CPD/450mL/<=-18C Irradiated Frozen <=6h	E3863
FRESH FROZEN PLASMA CPD/450mL/<=-18C Irradiated ResLeu:<1log6 Frozen <=6h	E3869
FRESH FROZEN PLASMA CPD/450mL/<=-18C ResLeu:<1log6 Frozen <=6h	E3866
FRESH FROZEN PLASMA CPD/450mL/<-25C For mnf:injectable Frozen <=24h	E3873
FRESH FROZEN PLASMA CPD/450mL/<-25C For mnf:injectable Frozen <=6h	E3858
FRESH FROZEN PLASMA CPD/450mL/<-25C For mnf:noninjectable Frozen <=6h	E3861
FRESH FROZEN PLASMA CPD/450mL/<-25C Frozen <=6h	E3855
FRESH FROZEN PLASMA CPD/450mL/<-25C Irradiated Frozen <=6h	E3864
FRESH FROZEN PLASMA CPD/450mL/<-25C Irradiated ResLeu:<1log6 Frozen <=6h.....	E3870
FRESH FROZEN PLASMA CPD/450mL/<-25C ResLeu:<1log6 Frozen <=6h.....	E3867
FRESH FROZEN PLASMA CPD/450mL/<-30 ResLeu:<1log6 Frozen <=6h.....	E3868

<u>Product Description</u>	<u>Product Code</u>
FRESH FROZEN PLASMA CPD/450mL/<-30C For mnf:injectable Frozen <=24h	E3874
FRESH FROZEN PLASMA CPD/450mL/<-30C For mnf:injectable Frozen <=6h	E3859
FRESH FROZEN PLASMA CPD/450mL/<-30C For mnf:noninjectable Frozen <=6h	E3862
FRESH FROZEN PLASMA CPD/450mL/<-30C Frozen <=6h	E3856
FRESH FROZEN PLASMA CPD/450mL/<-30C Irradiated Frozen <=6h	E3865
FRESH FROZEN PLASMA CPD/450mL/<-30C Irradiated ResLeu:<1log6 Frozen <=6h.....	E3871
FRESH FROZEN PLASMA CPD/XX/<=-18C.....	E0701
FRESH FROZEN PLASMA CPD/XX/<=-18C Irradiated.....	E0704
FRESH FROZEN PLASMA CPD/XX/<=-18C Not for tx or mnf.....	E0702
FRESH FROZEN PLASMA CPD/XX/<-65C	E0731
FRESH FROZEN PLASMA CPD/XX/<-65C Irradiated	E0734
FRESH FROZEN PLASMA CPD/XX/<-65C Not for tx or mnf.....	E0732
FRESH FROZEN PLASMA CPDA-1/XX/<=-18C	E0707
FRESH FROZEN PLASMA CPDA-1/XX/<=-18C Irradiated	E0710
FRESH FROZEN PLASMA CPDA-1/XX/<=-18C Not for tx or mnf	E0708
FRESH FROZEN PLASMA CPDA-1/XX/<-65C	E0737
FRESH FROZEN PLASMA CPDA-1/XX/<-65C Irradiated	E0740
FRESH FROZEN PLASMA CPDA-1/XX/<-65C Not for tx or mnf	E0738
FRESH FROZEN PLASMA NS/450mL/<-30C	E3821
FRESH FROZEN PLASMA NS/450mL/<-30C For mnf:noninjectable	E3838
FRESH FROZEN PLASMA NS/XX/<-30C ResLeu:<5log6	E4005
Frozen APHERESIS PLATELETS DMSO/XX/<-65C For mnf:injectable Open	E3447
Frozen APHERESIS PLATELETS DMSO/XX/<-65C For mnf:noninjectable Open	E3448
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Not for tx or mnf Open.....	E3449
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Not for tx or mnf Open 1st container	E3451
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Not for tx or mnf Open 1st container:not auto.....	E3455
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Not for tx or mnf Open 2nd container	E3452
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Not for tx or mnf Open 2nd container:not auto	E3456
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Not for tx or mnf Open 3rd container	E3453
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Not for tx or mnf Open 4th container	E3454

<u>Product Description</u>	<u>Product Code</u>
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Not for tx or mnf Open Aphr not automated	E3450
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Open	E3457
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Open 1st container.....	E3459
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Open 1st container:not auto	E3463
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Open 2nd container.....	E3460
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Open 2nd container:not auto.....	E3464
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Open 3rd container.....	E3461
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Open 4th container.....	E3462
Frozen APHERESIS PLATELETS DMSO/XX/<-65C Open Aphr not automated	E3458
Frozen POOLED SERUM None/450mL/<-30C For mnf:injectable Frozen >24h From 3 donors.....	E3986
Frozen RED BLOOD CELLS None/250mL/<-65C Not for tx or mnf Open	E0507
Frozen RED BLOOD CELLS None/250mL/<-65C Open	E0508
Frozen RED BLOOD CELLS None/250mL/<-65C Open Irradiated	E0509
Frozen RED BLOOD CELLS None/450mL/<-120C Not for tx or mnf Open.....	E0510
Frozen RED BLOOD CELLS None/450mL/<-120C Open	E0511
Frozen RED BLOOD CELLS None/450mL/<-120C Open Irradiated	E0512
Frozen RED BLOOD CELLS None/450mL/<-30C For mnf:injectable ResLeu:<1.2log9 Supernat rem	E3941
Frozen RED BLOOD CELLS None/450mL/<-65C Not for tx or mnf Open	E0501
Frozen RED BLOOD CELLS None/450mL/<-65C Open	E0502
Frozen RED BLOOD CELLS None/450mL/<-65C Open Irradiated	E0503
Frozen RED BLOOD CELLS None/500mL/<-65C Not for tx or mnf Open	E0504
Frozen RED BLOOD CELLS None/500mL/<-65C Open	E0505
Frozen RED BLOOD CELLS None/500mL/<-65C Open Irradiated	E0506
Frozen Rejuvenated RED BLOOD CELLS None/250mL/<-65C Not for tx or mnf Open	E0519
Frozen Rejuvenated RED BLOOD CELLS None/250mL/<-65C Open	E0520
Frozen Rejuvenated RED BLOOD CELLS None/250mL/<-65C Open Irradiated	E0521
Frozen Rejuvenated RED BLOOD CELLS None/450mL/<-120C Not for tx or mnf Open	E0522
Frozen Rejuvenated RED BLOOD CELLS None/450mL/<-120C Open	E0523
Frozen Rejuvenated RED BLOOD CELLS None/450mL/<-120C Open Irradiated	E0524
Frozen Rejuvenated RED BLOOD CELLS None/450mL/<-65C Not for tx or mnf Open	E0513

<u>Product Description</u>	<u>Product Code</u>
Frozen Rejuvenated RED BLOOD CELLS None/450mL/<-65C Open	E0514
Frozen Rejuvenated RED BLOOD CELLS None/450mL/<-65C Open Irradiated	E0515
Frozen Rejuvenated RED BLOOD CELLS None/500mL/<-65C Not for tx or mnf Open	E0516
Frozen Rejuvenated RED BLOOD CELLS None/500mL/<-65C Open	E0517
Frozen Rejuvenated RED BLOOD CELLS None/500mL/<-65C Open Irradiated	E0518
GRANULOCYTES CP2D/450mL/rt	E3649
GRANULOCYTES CP2D/450mL/rt Granulocytes prep: HES	E3660
GRANULOCYTES CP2D/450mL/rt Irradiated	E3658
GRANULOCYTES CP2D/450mL/rt Irradiated Granulocytes prep: HES	E3659
GRANULOCYTES CP2D/450mL/rt Not for tx or mnf	E3650
GRANULOCYTES CP2D/450mL/rt Not for tx or mnf Granulocytes prep: HES	E3653
GRANULOCYTES CP2D/450mL/rt Not for tx or mnf Irradiated	E3651
GRANULOCYTES CP2D/450mL/rt Not for tx or mnf Irradiated Granulocytes prep: HES	E3652
GRANULOCYTES CP2D/450mL/rt Open	E3654
GRANULOCYTES CP2D/450mL/rt Open Granulocytes prep: HES	E3657
GRANULOCYTES CP2D/450mL/rt Open Irradiated	E3655
GRANULOCYTES CP2D/450mL/rt Open Irradiated Granulocytes prep: HES	E3656
GRANULOCYTES CP2D/500mL/rt	E3661
GRANULOCYTES CP2D/500mL/rt Granulocytes prep: HES	E3672
GRANULOCYTES CP2D/500mL/rt Irradiated	E3670
GRANULOCYTES CP2D/500mL/rt Irradiated Granulocytes prep: HES	E3671
GRANULOCYTES CP2D/500mL/rt Not for tx or mnf	E3662
GRANULOCYTES CP2D/500mL/rt Not for tx or mnf Granulocytes prep: HES	E3665
GRANULOCYTES CP2D/500mL/rt Not for tx or mnf Irradiated	E3663
GRANULOCYTES CP2D/500mL/rt Not for tx or mnf Irradiated Granulocytes prep: HES	E3664
GRANULOCYTES CP2D/500mL/rt Open	E3666
GRANULOCYTES CP2D/500mL/rt Open Granulocytes prep: HES	E3669
GRANULOCYTES CP2D/500mL/rt Open Irradiated	E3667
GRANULOCYTES CP2D/500mL/rt Open Irradiated Granulocytes prep: HES	E3668
GRANULOCYTES CPD/450mL/rt	E3601

Product Description

Product Code

GRANULOCYTES CPD/450mL/rt Granulocytes prep: HES	E3612
GRANULOCYTES CPD/450mL/rt Irradiated	E3610
GRANULOCYTES CPD/450mL/rt Irradiated Granulocytes prep: HES	E3611
GRANULOCYTES CPD/450mL/rt Not for tx or mnf.....	E3602
GRANULOCYTES CPD/450mL/rt Not for tx or mnf Granulocytes prep: HES.....	E3605
GRANULOCYTES CPD/450mL/rt Not for tx or mnf Irradiated	E3603
GRANULOCYTES CPD/450mL/rt Not for tx or mnf Irradiated Granulocytes prep: HES.....	E3604
GRANULOCYTES CPD/450mL/rt Open.....	E3606
GRANULOCYTES CPD/450mL/rt Open Granulocytes prep: HES.....	E3609
GRANULOCYTES CPD/450mL/rt Open Irradiated.....	E3607
GRANULOCYTES CPD/450mL/rt Open Irradiated Granulocytes prep: HES.....	E3608
GRANULOCYTES CPD/500mL/rt	E3613
GRANULOCYTES CPD/500mL/rt Granulocytes prep: HES	E3624
GRANULOCYTES CPD/500mL/rt Irradiated	E3622
GRANULOCYTES CPD/500mL/rt Irradiated Granulocytes prep: HES	E3623
GRANULOCYTES CPD/500mL/rt Not for tx or mnf	E3614
GRANULOCYTES CPD/500mL/rt Not for tx or mnf Granulocytes prep: HES	E3617
GRANULOCYTES CPD/500mL/rt Not for tx or mnf Irradiated	E3615
GRANULOCYTES CPD/500mL/rt Not for tx or mnf Irradiated Granulocytes prep: HES	E3616
GRANULOCYTES CPD/500mL/rt Open.....	E3618
GRANULOCYTES CPD/500mL/rt Open Granulocytes prep: HES.....	E3621
GRANULOCYTES CPD/500mL/rt Open Irradiated.....	E3619
GRANULOCYTES CPD/500mL/rt Open Irradiated Granulocytes prep: HES.....	E3620
GRANULOCYTES CPDA-1/450mL/rt	E3625
GRANULOCYTES CPDA-1/450mL/rt Granulocytes prep: HES	E3636
GRANULOCYTES CPDA-1/450mL/rt Irradiated	E3634
GRANULOCYTES CPDA-1/450mL/rt Irradiated Granulocytes prep: HES	E3635
GRANULOCYTES CPDA-1/450mL/rt Not for tx or mnf	E3626
GRANULOCYTES CPDA-1/450mL/rt Not for tx or mnf Granulocytes prep: HES	E3629
GRANULOCYTES CPDA-1/450mL/rt Not for tx or mnf Irradiated	E3627

Product Description

Product Code

GRANULOCYTES CPDA-1/450mL/rt Not for tx or mnf Irradiated Granulocytes prep: HES	E3628
GRANULOCYTES CPDA-1/450mL/rt Open	E3630
GRANULOCYTES CPDA-1/450mL/rt Open Granulocytes prep: HES	E3633
GRANULOCYTES CPDA-1/450mL/rt Open Irradiated	E3631
GRANULOCYTES CPDA-1/450mL/rt Open Irradiated Granulocytes prep: HES	E3632
GRANULOCYTES CPDA-1/500mL/rt	E3637
GRANULOCYTES CPDA-1/500mL/rt Granulocytes prep: HES	E3648
GRANULOCYTES CPDA-1/500mL/rt Irradiated	E3646
GRANULOCYTES CPDA-1/500mL/rt Irradiated Granulocytes prep: HES	E3647
GRANULOCYTES CPDA-1/500mL/rt Not for tx or mnf	E3638
GRANULOCYTES CPDA-1/500mL/rt Not for tx or mnf Granulocytes prep: HES	E3641
GRANULOCYTES CPDA-1/500mL/rt Not for tx or mnf Irradiated	E3639
GRANULOCYTES CPDA-1/500mL/rt Not for tx or mnf Irradiated Granulocytes prep: HES	E3640
GRANULOCYTES CPDA-1/500mL/rt Open	E3642
GRANULOCYTES CPDA-1/500mL/rt Open Granulocytes prep: HES	E3645
GRANULOCYTES CPDA-1/500mL/rt Open Irradiated	E3643
GRANULOCYTES CPDA-1/500mL/rt Open Irradiated Granulocytes prep: HES	E3644
LEUKOCYTES CP2D/450mL/refg	E3717
LEUKOCYTES CP2D/450mL/refg For mnf:injectable	E3718
LEUKOCYTES CP2D/450mL/refg For mnf:noninjectable	E3719
LEUKOCYTES CP2D/450mL/refg Not for tx or mnf	E3720
LEUKOCYTES CP2D/450mL/refg Open	E3721
LEUKOCYTES CP2D/450mL/rt	E3747
LEUKOCYTES CP2D/450mL/rt For mnf:injectable	E3748
LEUKOCYTES CP2D/450mL/rt For mnf:noninjectable	E3749
LEUKOCYTES CP2D/450mL/rt Not for tx or mnf	E3750
LEUKOCYTES CP2D/450mL/rt Open	E3751
LEUKOCYTES CP2D/500mL/refg	E3722
LEUKOCYTES CP2D/500mL/refg For mnf:injectable	E3723
LEUKOCYTES CP2D/500mL/refg For mnf:noninjectable	E3724

<u>Product Description</u>	<u>Product Code</u>
LEUKOCYTES CP2D/500mL/refg Not for tx or mnf	E3725
LEUKOCYTES CP2D/500mL/refg Open	E3726
LEUKOCYTES CP2D/500mL/rt	E3752
LEUKOCYTES CP2D/500mL/rt For mnf:injectable	E3753
LEUKOCYTES CP2D/500mL/rt For mnf:noninjectable.....	E3754
LEUKOCYTES CP2D/500mL/rt Not for tx or mnf.....	E3755
LEUKOCYTES CP2D/500mL/rt Open.....	E3756
LEUKOCYTES CPD/450mL/refg.....	E3697
LEUKOCYTES CPD/450mL/refg For mnf:injectable.....	E3698
LEUKOCYTES CPD/450mL/refg For mnf:noninjectable	E3699
LEUKOCYTES CPD/450mL/refg Not for tx or mnf	E3700
LEUKOCYTES CPD/450mL/refg Open	E3701
LEUKOCYTES CPD/450mL/rt	E3727
LEUKOCYTES CPD/450mL/rt For mnf:injectable	E3728
LEUKOCYTES CPD/450mL/rt For mnf:noninjectable	E3729
LEUKOCYTES CPD/450mL/rt Not for tx or mnf	E3730
LEUKOCYTES CPD/450mL/rt Open	E3731
LEUKOCYTES CPD/500mL/refg.....	E3702
LEUKOCYTES CPD/500mL/refg For mnf:injectable.....	E3703
LEUKOCYTES CPD/500mL/refg For mnf:noninjectable	E3704
LEUKOCYTES CPD/500mL/refg Not for tx or mnf	E3705
LEUKOCYTES CPD/500mL/refg Open	E3706
LEUKOCYTES CPD/500mL/rt	E3732
LEUKOCYTES CPD/500mL/rt For mnf:injectable	E3733
LEUKOCYTES CPD/500mL/rt For mnf:noninjectable	E3734
LEUKOCYTES CPD/500mL/rt Not for tx or mnf	E3735
LEUKOCYTES CPD/500mL/rt Open	E3736
LEUKOCYTES CPDA-1/450mL/refg	E3707
LEUKOCYTES CPDA-1/450mL/refg For mnf:injectable	E3708
LEUKOCYTES CPDA-1/450mL/refg For mnf:noninjectable	E3709

<u>Product Description</u>	<u>Product Code</u>
LEUKOCYTES CPDA-1/450mL/refg Not for tx or mnf.....	E3710
LEUKOCYTES CPDA-1/450mL/refg Open	E3711
LEUKOCYTES CPDA-1/450mL/rt	E3737
LEUKOCYTES CPDA-1/450mL/rt For mnf:injectable	E3738
LEUKOCYTES CPDA-1/450mL/rt For mnf:noninjectable.....	E3739
LEUKOCYTES CPDA-1/450mL/rt Not for tx or mnf.....	E3740
LEUKOCYTES CPDA-1/450mL/rt Open.....	E3741
LEUKOCYTES CPDA-1/500mL/refg	E3712
LEUKOCYTES CPDA-1/500mL/refg For mnf:injectable	E3713
LEUKOCYTES CPDA-1/500mL/refg For mnf:noninjectable	E3714
LEUKOCYTES CPDA-1/500mL/refg Not for tx or mnf.....	E3715
LEUKOCYTES CPDA-1/500mL/refg Open	E3716
LEUKOCYTES CPDA-1/500mL/rt	E3742
LEUKOCYTES CPDA-1/500mL/rt For mnf:injectable	E3743
LEUKOCYTES CPDA-1/500mL/rt For mnf:noninjectable.....	E3744
LEUKOCYTES CPDA-1/500mL/rt Not for tx or mnf.....	E3745
LEUKOCYTES CPDA-1/500mL/rt Open.....	E3746
Liquid APHERESIS PLASMA ACD-A/XX/refg.....	E3813
Liquid APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf	E3814
Liquid APHERESIS PLASMA ACD-B/XX/refg.....	E3811
Liquid APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf	E3812
Liquid APHERESIS PLASMA NaCitrate/XX/refg	E3815
Liquid APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf	E3816
Liquid PLASMA CP2D/XX/<37C For mnf:injectable.....	E2493
Liquid PLASMA CP2D/XX/<37C For mnf:noninjectable.....	E2494
Liquid PLASMA CP2D/XX/<37C Not for tx or mnf	E2495
Liquid PLASMA CP2D/XX/refg.....	E2469
Liquid PLASMA CP2D/XX/refg Irradiated.....	E2474
Liquid PLASMA CP2D/XX/refg Not for tx or mnf	E2470
Liquid PLASMA CP2D/XX/refg Not for tx or mnf Open	E2471

<u>Product Description</u>	<u>Product Code</u>
Liquid PLASMA CP2D/XX/refg Open.....	E2472
Liquid PLASMA CP2D/XX/refg Open Irradiated.....	E2473
Liquid PLASMA CPD/450mL/refg	E3853
Liquid PLASMA CPD/XX/<37C For mnf:injectable	E2487
Liquid PLASMA CPD/XX/<37C For mnf:noninjectable	E2488
Liquid PLASMA CPD/XX/<37C Not for tx or mnf	E2489
Liquid PLASMA CPD/XX/refg	E2457
Liquid PLASMA CPD/XX/refg Irradiated	E2462
Liquid PLASMA CPD/XX/refg Not for tx or mnf	E2458
Liquid PLASMA CPD/XX/refg Not for tx or mnf Open.....	E2459
Liquid PLASMA CPD/XX/refg Open	E2460
Liquid PLASMA CPD/XX/refg Open Irradiated	E2461
Liquid PLASMA CPDA-1/XX/<37C For mnf:injectable.....	E2490
Liquid PLASMA CPDA-1/XX/<37C For mnf:noninjectable	E2491
Liquid PLASMA CPDA-1/XX/<37C Not for tx or mnf	E2492
Liquid PLASMA CPDA-1/XX/refg.....	E2463
Liquid PLASMA CPDA-1/XX/refg Irradiated.....	E2468
Liquid PLASMA CPDA-1/XX/refg Not for tx or mnf	E2464
Liquid PLASMA CPDA-1/XX/refg Not for tx or mnf Open	E2465
Liquid PLASMA CPDA-1/XX/refg Open	E2466
Liquid PLASMA CPDA-1/XX/refg Open Irradiated	E2467
PLASMA CP2D/XX/<=-18C	E2592
PLASMA CP2D/XX/<=-18C Cryo reduced	E2617
PLASMA CP2D/XX/<=-18C For mnf:injectable	E2593
PLASMA CP2D/XX/<=-18C For mnf:injectable Frozen <=24h.....	E2598
PLASMA CP2D/XX/<=-18C For mnf:injectable Frozen >24h	E2600
PLASMA CP2D/XX/<=-18C For mnf:injectable Irradiated	E2594
PLASMA CP2D/XX/<=-18C For mnf:injectable Irradiated Frozen <=24h.....	E2595
PLASMA CP2D/XX/<=-18C For mnf:noninjectable.....	E2603
PLASMA CP2D/XX/<=-18C For mnf:noninjectable Frozen <=24h.....	E2604

<u>Product Description</u>	<u>Product Code</u>
PLASMA CP2D/XX/<=-18C For mnf:noninjectable Frozen >24h.....	E2606
PLASMA CP2D/XX/<=-18C Frozen <=24h.....	E2619
PLASMA CP2D/XX/<=-18C Frozen >24h	E2621
PLASMA CP2D/XX/<=-18C Irradiated	E2611
PLASMA CP2D/XX/<=-18C Irradiated Cryo reduced	E2612
PLASMA CP2D/XX/<=-18C Irradiated Frozen <=24h.....	E2614
PLASMA CP2D/XX/<=-18C Not for tx or mnf.....	E2609
PLASMA CPD/450mL/<-30C For mnf:injectable Frozen <=24h.....	E3947
PLASMA CPD/450mL/<-30C For mnf:injectable Frozen <=6h	E3946
PLASMA CPD/450mL/<-30C For mnf:injectable Frozen >24h.....	E3948
PLASMA CPD/XX/<=-18C	E2528
PLASMA CPD/XX/<=-18C Cryo reduced	E2553
PLASMA CPD/XX/<=-18C For mnf:injectable	E2529
PLASMA CPD/XX/<=-18C For mnf:injectable Frozen <=24h	E2534
PLASMA CPD/XX/<=-18C For mnf:injectable Frozen >24h	E2536
PLASMA CPD/XX/<=-18C For mnf:injectable Irradiated	E2530
PLASMA CPD/XX/<=-18C For mnf:injectable Irradiated Frozen <=24h	E2531
PLASMA CPD/XX/<=-18C For mnf:noninjectable	E2539
PLASMA CPD/XX/<=-18C For mnf:noninjectable Frozen <=24h	E2540
PLASMA CPD/XX/<=-18C For mnf:noninjectable Frozen >24h	E2542
PLASMA CPD/XX/<=-18C Frozen <=24h	E2555
PLASMA CPD/XX/<=-18C Frozen >24h	E2557
PLASMA CPD/XX/<=-18C Irradiated	E2547
PLASMA CPD/XX/<=-18C Irradiated Cryo reduced	E2548
PLASMA CPD/XX/<=-18C Irradiated Frozen <=24h	E2550
PLASMA CPD/XX/<=-18C Not for tx or mnf	E2545
PLASMA CPDA-1/XX/<=-18C.....	E2560
PLASMA CPDA-1/XX/<=-18C Cryo reduced	E2585
PLASMA CPDA-1/XX/<=-18C For mnf:injectable.....	E2561
PLASMA CPDA-1/XX/<=-18C For mnf:injectable Frozen <=24h.....	E2566

<u>Product Description</u>	<u>Product Code</u>
PLASMA CPDA-1/XX/<=-18C For mnf:injectable Frozen >24h	E2568
PLASMA CPDA-1/XX/<=-18C For mnf:injectable Irradiated.....	E2562
PLASMA CPDA-1/XX/<=-18C For mnf:injectable Irradiated Frozen <=24h.....	E2563
PLASMA CPDA-1/XX/<=-18C For mnf:noninjectable.....	E2571
PLASMA CPDA-1/XX/<=-18C For mnf:noninjectable Frozen <=24h	E2572
PLASMA CPDA-1/XX/<=-18C For mnf:noninjectable Frozen >24h.....	E2574
PLASMA CPDA-1/XX/<=-18C Frozen <=24h.....	E2587
PLASMA CPDA-1/XX/<=-18C Frozen >24h	E2589
PLASMA CPDA-1/XX/<=-18C Irradiated.....	E2579
PLASMA CPDA-1/XX/<=-18C Irradiated Cryo reduced	E2580
PLASMA CPDA-1/XX/<=-18C Irradiated Frozen <=24h.....	E2582
PLASMA CPDA-1/XX/<=-18C Not for tx or mnf.....	E2577
PLASMA NS/XX/<-30C ResLeu:<5log6	E4007
PLATELET-RICH BUFFY COAT CPD/450mL/20-24C	E3817
PLATELET-RICH BUFFY COAT CPD/450mL/20-24C For mnf:noninjectable	E3895
PLATELET-RICH BUFFY COAT CPD/450mL/20-24C Not for tx or mnf	E3818
PLATELET-RICH PLASMA CP2D/450mL/20-24C	E2782
PLATELET-RICH PLASMA CP2D/450mL/20-24C Not for tx or mnf	E2783
PLATELET-RICH PLASMA CP2D/500mL/20-24C	E2784
PLATELET-RICH PLASMA CP2D/500mL/20-24C Not for tx or mnf	E2785
PLATELET-RICH PLASMA CPD/450mL/20-24C.....	E2774
PLATELET-RICH PLASMA CPD/450mL/20-24C Not for tx or mnf	E2775
PLATELET-RICH PLASMA CPD/500mL/20-24C.....	E2776
PLATELET-RICH PLASMA CPD/500mL/20-24C Not for tx or mnf	E2777
PLATELET-RICH PLASMA CPD/450mL/20-24C	E2778
PLATELET-RICH PLASMA CPDA-1/450mL/20-24C Not for tx or mnf	E2779
PLATELET-RICH PLASMA CPDA-1/500mL/20-24C	E2780
PLATELET-RICH PLASMA CPDA-1/500mL/20-24C Not for tx or mnf	E2781
PLATELET-RICH PLASMA NS/450mL/20-24C.....	E2788
PLATELET-RICH PLASMA NS/450mL/20-24C Not for tx or mnf	E2789

<u>Product Description</u>	<u>Product Code</u>
PLATELETS CP2D/450mL/20-24C.....	E2851
PLATELETS CP2D/450mL/20-24C Irradiated.....	E2853
PLATELETS CP2D/450mL/20-24C Irradiated Plasma reduced	E2856
PLATELETS CP2D/450mL/20-24C Irradiated ResLeu:<8.3log5	E2854
PLATELETS CP2D/450mL/20-24C Irradiated ResLeu:<8.3log5 Plasma reduced	E2855
PLATELETS CP2D/450mL/20-24C Not for tx or mnf	E2852
PLATELETS CP2D/450mL/20-24C Plasma reduced.....	E2859
PLATELETS CP2D/450mL/20-24C ResLeu:<8.3log5	E2857
PLATELETS CP2D/450mL/20-24C ResLeu:<8.3log5 Plasma reduced	E2858
PLATELETS CP2D/500mL/20-24C.....	E2860
PLATELETS CP2D/500mL/20-24C Irradiated.....	E2862
PLATELETS CP2D/500mL/20-24C Irradiated Plasma reduced	E2865
PLATELETS CP2D/500mL/20-24C Irradiated ResLeu:<8.3log5	E2863
PLATELETS CP2D/500mL/20-24C Irradiated ResLeu:<8.3log5 Plasma reduced	E2864
PLATELETS CP2D/500mL/20-24C Not for tx or mnf	E2861
PLATELETS CP2D/500mL/20-24C Plasma reduced.....	E2868
PLATELETS CP2D/500mL/20-24C ResLeu:<8.3log5	E2866
PLATELETS CP2D/500mL/20-24C ResLeu:<8.3log5 Plasma reduced	E2867
PLATELETS CP2D/XX/<37C For mnf:injectable	E2804
PLATELETS CP2D/XX/<37C For mnf:noninjectable.....	E2805
PLATELETS CP2D/XX/<37C Not for tx or mnf.....	E2806
PLATELETS CPD/450mL/20-24C	E2807
PLATELETS CPD/450mL/20-24C Irradiated	E2809
PLATELETS CPD/450mL/20-24C Irradiated Plasma reduced	E2814
PLATELETS CPD/450mL/20-24C Irradiated ResLeu:<8.3log5.....	E2810
PLATELETS CPD/450mL/20-24C Irradiated ResLeu:<8.3log5 Plasma reduced.....	E2811
PLATELETS CPD/450mL/20-24C Not for tx or mnf.....	E2808
PLATELETS CPD/450mL/20-24C Plasma reduced	E2821
PLATELETS CPD/450mL/20-24C ResLeu:<8.3log5.....	E2817
PLATELETS CPD/450mL/20-24C ResLeu:<8.3log5 Plasma reduced.....	E2818

<u>Product Description</u>	<u>Product Code</u>
PLATELETS CPD/450mL/refg	E2790
PLATELETS CPD/450mL/refg For mnf:injectable	E2791
PLATELETS CPD/450mL/refg For mnf:noninjectable	E2792
PLATELETS CPD/450mL/refg Not for tx or mnf	E2793
PLATELETS CPD/500mL/20-24C	E2824
PLATELETS CPD/500mL/20-24C Irradiated	E2826
PLATELETS CPD/500mL/20-24C Irradiated Plasma reduced	E2829
PLATELETS CPD/500mL/20-24C Irradiated ResLeu:<8.3log5.....	E2827
PLATELETS CPD/500mL/20-24C Irradiated ResLeu:<8.3log5 Plasma reduced.....	E2828
PLATELETS CPD/500mL/20-24C Not for tx or mnf.....	E2825
PLATELETS CPD/500mL/20-24C Plasma reduced	E2832
PLATELETS CPD/500mL/20-24C ResLeu:<8.3log5.....	E2830
PLATELETS CPD/500mL/20-24C ResLeu:<8.3log5 Plasma reduced.....	E2831
PLATELETS CPD/XX/<37C For mnf:injectable	E2798
PLATELETS CPD/XX/<37C For mnf:noninjectable	E2799
PLATELETS CPD/XX/<37C Not for tx or mnf	E2800
PLATELETS CPDA-1/450mL/20-24C	E2833
PLATELETS CPDA-1/450mL/20-24C Irradiated	E2835
PLATELETS CPDA-1/450mL/20-24C Irradiated Plasma reduced	E2838
PLATELETS CPDA-1/450mL/20-24C Irradiated ResLeu:<8.3log5	E2836
PLATELETS CPDA-1/450mL/20-24C Irradiated ResLeu:<8.3log5 Plasma reduced	E2837
PLATELETS CPDA-1/450mL/20-24C Not for tx or mnf	E2834
PLATELETS CPDA-1/450mL/20-24C Plasma reduced	E2841
PLATELETS CPDA-1/450mL/20-24C ResLeu:<8.3log5	E2839
PLATELETS CPDA-1/450mL/20-24C ResLeu:<8.3log5 Plasma reduced	E2840
PLATELETS CPDA-1/450mL/refg	E2794
PLATELETS CPDA-1/450mL/refg For mnf:injectable	E2795
PLATELETS CPDA-1/450mL/refg For mnf:noninjectable	E2796
PLATELETS CPDA-1/450mL/refg Not for tx or mnf.....	E2797
PLATELETS CPDA-1/500mL/20-24C	E2842

<u>Product Description</u>	<u>Product Code</u>
PLATELETS CPDA-1/500mL/20-24C Irradiated	E2844
PLATELETS CPDA-1/500mL/20-24C Irradiated Plasma reduced	E2847
PLATELETS CPDA-1/500mL/20-24C Irradiated ResLeu:<8.3log5	E2845
PLATELETS CPDA-1/500mL/20-24C Irradiated ResLeu:<8.3log5 Plasma reduced	E2846
PLATELETS CPDA-1/500mL/20-24C Not for tx or mnf	E2843
PLATELETS CPDA-1/500mL/20-24C Plasma reduced	E2850
PLATELETS CPDA-1/500mL/20-24C ResLeu:<8.3log5	E2848
PLATELETS CPDA-1/500mL/20-24C ResLeu:<8.3log5 Plasma reduced	E2849
PLATELETS CPDA-1/XX/<37C For mnf:injectable	E2801
PLATELETS CPDA-1/XX/<37C For mnf:noninjectable	E2802
PLATELETS CPDA-1/XX/<37C Not for tx or mnf	E2803
PLATELETS NS/450mL/20-24C	E2885
PLATELETS NS/450mL/20-24C For mnf:injectable	E2886
PLATELETS NS/450mL/20-24C For mnf:noninjectable	E2887
PLATELETS NS/450mL/20-24C Irradiated Plasma reduced	E3841
PLATELETS NS/450mL/20-24C Not for tx or mnf	E2888
PLATELETS NS/450mL/20-24C Plasma reduced	E3840
PLATELETS NS/450mL/refg	E2869
PLATELETS NS/450mL/refg For mnf:injectable	E2870
PLATELETS NS/450mL/refg For mnf:noninjectable	E2871
PLATELETS NS/450mL/refg Not for tx or mnf	E2872
POOLED CRYOPRECIPITATE None/XX/<=-18C	E3587
POOLED CRYOPRECIPITATE None/XX/<=-18C Irradiated	E3590
POOLED CRYOPRECIPITATE None/XX/<=-18C Open	E3588
POOLED CRYOPRECIPITATE None/XX/<=-18C Open Irradiated	E3589
POOLED GRANULOCYTES CPD/450mL/rt Irradiated From 7 donors	E3987
POOLED GRANULOCYTES CPD/450mL/rt Irradiated From 8 donors	E3988
POOLED GRANULOCYTES CPD/450mL/rt Irradiated From 6 donors	E3967
POOLED GRANULOCYTES CPD/450mL/rt Irradiated ResLeu:<2log5 From 4 donors	E3989
POOLED GRANULOCYTES CPD/450mL/rt Irradiated ResLeu:<2log5 From 5 donors	E3990

Product Description

Product Code

POOLED GRANULOCYTES CPD/450mL/rt Irradiated ResLeu:<2log5 From 6 donors.....	E3991
POOLED GRANULOCYTES NS/XX/rt.....	E3679
POOLED GRANULOCYTES NS/XX/rt Granulocytes prep: HES.....	E3690
POOLED GRANULOCYTES NS/XX/rt Irradiated.....	E3688
POOLED GRANULOCYTES NS/XX/rt Irradiated Granulocytes prep: HES.....	E3689
POOLED GRANULOCYTES NS/XX/rt Not for tx or mnf	E3680
POOLED GRANULOCYTES NS/XX/rt Not for tx or mnf Granulocytes prep: HES	E3683
POOLED GRANULOCYTES NS/XX/rt Not for tx or mnf Open	E3681
POOLED GRANULOCYTES NS/XX/rt Not for tx or mnf Open Granulocytes prep: HES	E3682
POOLED GRANULOCYTES NS/XX/rt Open	E3684
POOLED GRANULOCYTES NS/XX/rt Open Granulocytes prep: HES	E3687
POOLED GRANULOCYTES NS/XX/rt Open Irradiated	E3685
POOLED GRANULOCYTES NS/XX/rt Open Irradiated Granulocytes prep: HES	E3686
POOLED PLASMA CPD/450mL/<-25C/For mnf:injectable/Frozen <=24h.....	E4014
POOLED PLASMA CPD/450mL/<-25C/Frozen <=6h	E4013
POOLED PLASMA CPD/450mL/<-30C Cryo reduced Frozen <=6h From 2 donors.....	E3985
POOLED PLASMA CPD/450mL/<-30C For mnf:injectable Frozen <=24h From 2 donors	E3983
POOLED PLASMA CPD/450mL/<-30C For mnf:injectable Frozen >24h From 2 donors	E3984
POOLED PLASMA CPD/450mL/<-30CFrozen <=6h From 2 donors	E3992
POOLED PLASMA NS/XX/<37C For mnf:injectable	E3805
POOLED PLASMA NS/XX/<37C For mnf:injectable Open	E3806
POOLED PLASMA NS/XX/<37C For mnf:noninjectable	E3807
POOLED PLASMA NS/XX/<37C For mnf:noninjectable Open	E3808
POOLED PLASMA NS/XX/<37C Not for tx or mnf	E3809
POOLED PLASMA NS/XX/<37C Not for tx or mnf Open	E3810
POOLED PLATELETS NS/XX/20-24C.....	E2897
POOLED PLATELETS NS/XX/20-24C For mnf:injectable	E2898
POOLED PLATELETS NS/XX/20-24C For mnf:noninjectable	E2899
POOLED PLATELETS NS/XX/20-24C Irradiated.....	E2910
POOLED PLATELETS NS/XX/20-24C Irradiated Plasma reduced	E2913

<u>Product Description</u>	<u>Product Code</u>
POOLED PLATELETS NS/XX/20-24C Irradiated ResLeu:<5log6	E2911
POOLED PLATELETS NS/XX/20-24C Irradiated ResLeu:<5log6 Plasma reduced	E2912
POOLED PLATELETS NS/XX/20-24C Not for tx or mnf	E2900
POOLED PLATELETS NS/XX/20-24C Not for tx or mnf Open	E2901
POOLED PLATELETS NS/XX/20-24C Open.....	E2902
POOLED PLATELETS NS/XX/20-24C Open Irradiated.....	E2903
POOLED PLATELETS NS/XX/20-24C Open Irradiated Plasma reduced.....	E2906
POOLED PLATELETS NS/XX/20-24C Open Irradiated ResLeu:<5log6	E2904
POOLED PLATELETS NS/XX/20-24C Open Irradiated ResLeu:<5log6 Plasma reduced.....	E2905
POOLED PLATELETS NS/XX/20-24C Open Plasma reduced	E2909
POOLED PLATELETS NS/XX/20-24C Open ResLeu:<5log6	E2907
POOLED PLATELETS NS/XX/20-24C Open ResLeu:<5log6 Plasma reduced.....	E2908
POOLED PLATELETS NS/XX/20-24C Plasma reduced	E2916
POOLED PLATELETS NS/XX/20-24C ResLeu:<5log6	E2914
POOLED PLATELETS NS/XX/20-24C ResLeu:<5log6 Plasma reduced	E2915
POOLED PLATELETS PASII/XX/20-24C ResLeu:<2log5 Supernat reduced Buffy coat plts prep From 4 donors	E3996
RED BLOOD CELLS AS1/450mL/refg.....	E0291
RED BLOOD CELLS AS1/450mL/refg For mnf:injectable	E0292
RED BLOOD CELLS AS1/450mL/refg For mnf:noninjectable	E0293
RED BLOOD CELLS AS1/450mL/refg Irradiated	E0306
RED BLOOD CELLS AS1/450mL/refg Irradiated Plasma added	E0308
RED BLOOD CELLS AS1/450mL/refg Irradiated ResLeu:<5log6	E0307
RED BLOOD CELLS AS1/450mL/refg Irradiated Supernat rem	E0309
RED BLOOD CELLS AS1/450mL/refg Irradiated Supernat rem/Plasma added	E0310
RED BLOOD CELLS AS1/450mL/refg Not for tx or mnf	E0294
RED BLOOD CELLS AS1/450mL/refg Open	E0295
RED BLOOD CELLS AS1/450mL/refg Open Albumin added	E0302
RED BLOOD CELLS AS1/450mL/refg Open Irradiated	E0296
RED BLOOD CELLS AS1/450mL/refg Open Irradiated Plasma added.....	E0298

<u>Product Description</u>	<u>Product Code</u>
RED BLOOD CELLS AS1/450mL/refg Open Irradiated ResLeu:<5log6.....	E0297
RED BLOOD CELLS AS1/450mL/refg Open Irradiated Supernat rem.....	E0299
RED BLOOD CELLS AS1/450mL/refg Open Irradiated Supernat rem/Plasma added	E0300
RED BLOOD CELLS AS1/450mL/refg Open Plasma added.....	E0303
RED BLOOD CELLS AS1/450mL/refg Open ResLeu:<5log6.....	E0301
RED BLOOD CELLS AS1/450mL/refg Open Supernat rem.....	E0304
RED BLOOD CELLS AS1/450mL/refg Open Supernat rem/Plasma added	E0305
RED BLOOD CELLS AS1/450mL/refg Plasma added	E0313
RED BLOOD CELLS AS1/450mL/refg ResLeu:<5log6	E0311
RED BLOOD CELLS AS1/450mL/refg Supernat rem	E0314
RED BLOOD CELLS AS1/450mL/refg Supernat rem/Plasma added	E0315
RED BLOOD CELLS AS1/500mL/refg.....	E0316
RED BLOOD CELLS AS1/500mL/refg For mnf:injectable	E0317
RED BLOOD CELLS AS1/500mL/refg For mnf:noninjectable	E0318
RED BLOOD CELLS AS1/500mL/refg Irradiated	E0331
RED BLOOD CELLS AS1/500mL/refg Irradiated Plasma added	E0333
RED BLOOD CELLS AS1/500mL/refg Irradiated ResLeu:<5log6	E0332
RED BLOOD CELLS AS1/500mL/refg Irradiated Supernat rem	E0334
RED BLOOD CELLS AS1/500mL/refg Irradiated Supernat rem/Plasma added	E0335
RED BLOOD CELLS AS1/500mL/refg Not for tx or mnf	E0319
RED BLOOD CELLS AS1/500mL/refg Open	E0320
RED BLOOD CELLS AS1/500mL/refg Open Albumin added	E0327
RED BLOOD CELLS AS1/500mL/refg Open Irradiated	E0321
RED BLOOD CELLS AS1/500mL/refg Open Irradiated Plasma added.....	E0323
RED BLOOD CELLS AS1/500mL/refg Open Irradiated ResLeu:<5log6.....	E0322
RED BLOOD CELLS AS1/500mL/refg Open Irradiated Supernat rem.....	E0324
RED BLOOD CELLS AS1/500mL/refg Open Irradiated Supernat rem/Plasma added	E0325
RED BLOOD CELLS AS1/500mL/refg Open Plasma added.....	E0328
RED BLOOD CELLS AS1/500mL/refg Open ResLeu:<5log6.....	E0326
RED BLOOD CELLS AS1/500mL/refg Open Supernat rem.....	E0329

<u>Product Description</u>	<u>Product Code</u>
RED BLOOD CELLS AS1/500mL/refg Open Supernat rem/Plasma added	E0330
RED BLOOD CELLS AS1/500mL/refg Plasma added	E0338
RED BLOOD CELLS AS1/500mL/refg ResLeu:<5log6	E0336
RED BLOOD CELLS AS1/500mL/refg Supernat rem	E0339
RED BLOOD CELLS AS1/500mL/refg Supernat rem/Plasma added	E0340
RED BLOOD CELLS AS1/XX/refg	E0462
RED BLOOD CELLS AS1/XX/refg Low volume	E0463
RED BLOOD CELLS AS3/450mL/refg	E0341
RED BLOOD CELLS AS3/450mL/refg For mnf:injectable	E0342
RED BLOOD CELLS AS3/450mL/refg For mnf:noninjectable	E0343
RED BLOOD CELLS AS3/450mL/refg Irradiated	E0356
RED BLOOD CELLS AS3/450mL/refg Irradiated Plasma added	E0358
RED BLOOD CELLS AS3/450mL/refg Irradiated ResLeu:<5log6	E0357
RED BLOOD CELLS AS3/450mL/refg Irradiated Supernat rem	E0359
RED BLOOD CELLS AS3/450mL/refg Irradiated Supernat rem/Plasma added	E0360
RED BLOOD CELLS AS3/450mL/refg Not for tx or mnf	E0344
RED BLOOD CELLS AS3/450mL/refg Open	E0345
RED BLOOD CELLS AS3/450mL/refg Open Albumin added	E0352
RED BLOOD CELLS AS3/450mL/refg Open Irradiated	E0346
RED BLOOD CELLS AS3/450mL/refg Open Irradiated Plasma added	E0348
RED BLOOD CELLS AS3/450mL/refg Open Irradiated ResLeu:<5log6	E0347
RED BLOOD CELLS AS3/450mL/refg Open Irradiated Supernat rem	E0349
RED BLOOD CELLS AS3/450mL/refg Open Irradiated Supernat rem/Plasma added	E0350
RED BLOOD CELLS AS3/450mL/refg Open Plasma added	E0353
RED BLOOD CELLS AS3/450mL/refg Open ResLeu:<5log6	E0351
RED BLOOD CELLS AS3/450mL/refg Open Supernat rem	E0354
RED BLOOD CELLS AS3/450mL/refg Open Supernat rem/Plasma added	E0355
RED BLOOD CELLS AS3/450mL/refg Plasma added	E0363
RED BLOOD CELLS AS3/450mL/refg ResLeu:<5log6	E0361
RED BLOOD CELLS AS3/450mL/refg Supernat rem	E0364

Product Description

Product Code

RED BLOOD CELLS AS3/450mL/refg Supernat rem/Plasma added	E0365
RED BLOOD CELLS AS3/500mL/refg.....	E0366
RED BLOOD CELLS AS3/500mL/refg For mnf:injectable	E0367
RED BLOOD CELLS AS3/500mL/refg For mnf:noninjectable	E0368
RED BLOOD CELLS AS3/500mL/refg Irradiated.....	E0378
RED BLOOD CELLS AS3/500mL/refg Irradiated ResLeu:<5log6	E0379
RED BLOOD CELLS AS3/500mL/refg Irradiated Supernat rem	E0380
RED BLOOD CELLS AS3/500mL/refg Irradiated Supernat rem/Plasma added	E0381
RED BLOOD CELLS AS3/500mL/refg Not for tx or mnf	E0369
RED BLOOD CELLS AS3/500mL/refg Open	E0370
RED BLOOD CELLS AS3/500mL/refg Open Irradiated	E0371
RED BLOOD CELLS AS3/500mL/refg Open Irradiated ResLeu:<5log6.....	E0372
RED BLOOD CELLS AS3/500mL/refg Open Irradiated Supernat rem.....	E0373
RED BLOOD CELLS AS3/500mL/refg Open Irradiated Supernat rem/Plasma added	E0374
RED BLOOD CELLS AS3/500mL/refg Open ResLeu:<5log6.....	E0375
RED BLOOD CELLS AS3/500mL/refg Open Supernat rem.....	E0376
RED BLOOD CELLS AS3/500mL/refg Open Supernat rem/Plasma added	E0377
RED BLOOD CELLS AS3/500mL/refg ResLeu:<5log6	E0382
RED BLOOD CELLS AS3/500mL/refg Supernat rem	E0383
RED BLOOD CELLS AS3/500mL/refg Supernat rem/Plasma added	E0384
RED BLOOD CELLS AS3/XX/refg	E0464
RED BLOOD CELLS AS3/XX/refg Low volume.....	E0465
RED BLOOD CELLS AS5/450mL/refg.....	E0385
RED BLOOD CELLS AS5/450mL/refg For mnf:injectable	E0386
RED BLOOD CELLS AS5/450mL/refg For mnf:noninjectable	E0387
RED BLOOD CELLS AS5/450mL/refg Irradiated	E0397
RED BLOOD CELLS AS5/450mL/refg Irradiated ResLeu:<5log6	E0398
RED BLOOD CELLS AS5/450mL/refg Irradiated Supernat rem	E0399
RED BLOOD CELLS AS5/450mL/refg Irradiated Supernat rem/Plasma added	E0400
RED BLOOD CELLS AS5/450mL/refg Not for tx or mnf	E0388

<u>Product Description</u>	<u>Product Code</u>
RED BLOOD CELLS AS5/450mL/refg Open	E0389
RED BLOOD CELLS AS5/450mL/refg Open Irradiated	E0390
RED BLOOD CELLS AS5/450mL/refg Open Irradiated ResLeu:<5log6.....	E0391
RED BLOOD CELLS AS5/450mL/refg Open Irradiated Supernat rem.....	E0392
RED BLOOD CELLS AS5/450mL/refg Open Irradiated Supernat rem/Plasma added	E0393
RED BLOOD CELLS AS5/450mL/refg Open ResLeu:<5log6.....	E0394
RED BLOOD CELLS AS5/450mL/refg Open Supernat rem.....	E0395
RED BLOOD CELLS AS5/450mL/refg Open Supernat rem/Plasma added	E0396
RED BLOOD CELLS AS5/450mL/refg ResLeu:<5log6	E0401
RED BLOOD CELLS AS5/450mL/refg Supernat rem	E0402
RED BLOOD CELLS AS5/450mL/refg Supernat rem/Plasma added	E0403
RED BLOOD CELLS AS5/500mL/refg.....	E0404
RED BLOOD CELLS AS5/500mL/refg For mnf:injectable	E0405
RED BLOOD CELLS AS5/500mL/refg For mnf:noninjectable	E0406
RED BLOOD CELLS AS5/500mL/refg Irradiated	E0419
RED BLOOD CELLS AS5/500mL/refg Irradiated Plasma added	E0421
RED BLOOD CELLS AS5/500mL/refg Irradiated ResLeu:<5log6	E0420
RED BLOOD CELLS AS5/500mL/refg Irradiated Supernat rem	E0422
RED BLOOD CELLS AS5/500mL/refg Irradiated Supernat rem/Plasma added	E0423
RED BLOOD CELLS AS5/500mL/refg Not for tx or mnf	E0407
RED BLOOD CELLS AS5/500mL/refg Open	E0408
RED BLOOD CELLS AS5/500mL/refg Open Albumin added	E0415
RED BLOOD CELLS AS5/500mL/refg Open Irradiated	E0409
RED BLOOD CELLS AS5/500mL/refg Open Irradiated Plasma added.....	E0411
RED BLOOD CELLS AS5/500mL/refg Open Irradiated ResLeu:<5log6.....	E0410
RED BLOOD CELLS AS5/500mL/refg Open Irradiated Supernat rem.....	E0412
RED BLOOD CELLS AS5/500mL/refg Open Irradiated Supernat rem/Plasma added	E0413
RED BLOOD CELLS AS5/500mL/refg Open Plasma added.....	E0416
RED BLOOD CELLS AS5/500mL/refg Open ResLeu:<5log6.....	E0414
RED BLOOD CELLS AS5/500mL/refg Open Supernat rem.....	E0417

<u>Product Description</u>	<u>Product Code</u>
RED BLOOD CELLS AS5/500mL/refg Open Supernat rem/Plasma added	E0418
RED BLOOD CELLS AS5/500mL/refg Plasma added	E0426
RED BLOOD CELLS AS5/500mL/refg ResLeu:<5log6	E0424
RED BLOOD CELLS AS5/500mL/refg Supernat rem	E0427
RED BLOOD CELLS AS5/500mL/refg Supernat rem/Plasma added	E0428
RED BLOOD CELLS AS5/XX/refg	E0466
RED BLOOD CELLS AS5/XX/refg Low volume.....	E0467
RED BLOOD CELLS CP2D/450mL/refg.....	E0245
RED BLOOD CELLS CP2D/450mL/refg For mnf:injectable.....	E0246
RED BLOOD CELLS CP2D/450mL/refg For mnf:noninjectable.....	E0247
RED BLOOD CELLS CP2D/450mL/refg Irradiated.....	E0256
RED BLOOD CELLS CP2D/450mL/refg Irradiated Plasma added	E0258
RED BLOOD CELLS CP2D/450mL/refg Irradiated ResLeu:<5log6	E0257
RED BLOOD CELLS CP2D/450mL/refg Not for tx or mnf	E0248
RED BLOOD CELLS CP2D/450mL/refg Open.....	E0249
RED BLOOD CELLS CP2D/450mL/refg Open Albumin added.....	E0254
RED BLOOD CELLS CP2D/450mL/refg Open Irradiated.....	E0250
RED BLOOD CELLS CP2D/450mL/refg Open Irradiated Plasma added	E0252
RED BLOOD CELLS CP2D/450mL/refg Open Irradiated ResLeu:<5log6	E0251
RED BLOOD CELLS CP2D/450mL/refg Open Plasma added	E0255
RED BLOOD CELLS CP2D/450mL/refg Open ResLeu:<5log6	E0253
RED BLOOD CELLS CP2D/450mL/refg Plasma added	E0261
RED BLOOD CELLS CP2D/450mL/refg ResLeu:<5log6	E0259
RED BLOOD CELLS CP2D/500mL/refg.....	E0262
RED BLOOD CELLS CP2D/500mL/refg For mnf:injectable.....	E0263
RED BLOOD CELLS CP2D/500mL/refg For mnf:noninjectable.....	E0264
RED BLOOD CELLS CP2D/500mL/refg Irradiated.....	E0273
RED BLOOD CELLS CP2D/500mL/refg Irradiated Plasma added	E0275
RED BLOOD CELLS CP2D/500mL/refg Irradiated ResLeu:<5log6	E0274
RED BLOOD CELLS CP2D/500mL/refg Not for tx or mnf	E0265

Product Description

Product Code

RED BLOOD CELLS CP2D/500mL/refg Open.....	E0266
RED BLOOD CELLS CP2D/500mL/refg Open Albumin added.....	E0271
RED BLOOD CELLS CP2D/500mL/refg Open Irradiated.....	E0267
RED BLOOD CELLS CP2D/500mL/refg Open Irradiated Plasma added	E0269
RED BLOOD CELLS CP2D/500mL/refg Open Irradiated ResLeu:<5log6	E0268
RED BLOOD CELLS CP2D/500mL/refg Open Plasma added	E0272
RED BLOOD CELLS CP2D/500mL/refg Open ResLeu:<5log6	E0270
RED BLOOD CELLS CP2D/500mL/refg Plasma added	E0278
RED BLOOD CELLS CP2D/500mL/refg ResLeu:<5log6	E0276
RED BLOOD CELLS CP2D/XX/refg.....	E0279
RED BLOOD CELLS CP2D/XX/refg For mnf:injectable.....	E0280
RED BLOOD CELLS CP2D/XX/refg For mnf:noninjectable	E0281
RED BLOOD CELLS CP2D/XX/refg Low volume.....	E0283
RED BLOOD CELLS CP2D/XX/refg Not for tx or mnf	E0282
RED BLOOD CELLS CPD/250mL/refg	E0184
RED BLOOD CELLS CPD/250mL/refg For mnf:injectable	E0185
RED BLOOD CELLS CPD/250mL/refg For mnf:noninjectable	E0186
RED BLOOD CELLS CPD/250mL/refg Irradiated	E0188
RED BLOOD CELLS CPD/250mL/refg Irradiated ResLeu:<5log6	E0189
RED BLOOD CELLS CPD/250mL/refg Not for tx or mnf.....	E0187
RED BLOOD CELLS CPD/250mL/refg ResLeu:<5log6.....	E0190
RED BLOOD CELLS CPD/450mL/refg	E0150
RED BLOOD CELLS CPD/450mL/refg For mnf:injectable	E0151
RED BLOOD CELLS CPD/450mL/refg For mnf:noninjectable	E0152
RED BLOOD CELLS CPD/450mL/refg Irradiated	E0161
RED BLOOD CELLS CPD/450mL/refg Irradiated Plasma added.....	E0163
RED BLOOD CELLS CPD/450mL/refg Irradiated ResLeu:<1log6 Plts/Cryo reduced	E3938
RED BLOOD CELLS CPD/450mL/refg Irradiated ResLeu:<5log6	E0162
RED BLOOD CELLS CPD/450mL/refg Not for tx or mnf.....	E0153
RED BLOOD CELLS CPD/450mL/refg Open	E0154

<u>Product Description</u>	<u>Product Code</u>
RED BLOOD CELLS CPD/450mL/refg Open Albumin added	E0159
RED BLOOD CELLS CPD/450mL/refg Open Irradiated	E0155
RED BLOOD CELLS CPD/450mL/refg Open Irradiated Plasma added	E0157
RED BLOOD CELLS CPD/450mL/refg Open Irradiated ResLeu:<5log6	E0156
RED BLOOD CELLS CPD/450mL/refg Open Plasma added	E0160
RED BLOOD CELLS CPD/450mL/refg Open ResLeu:<5log6	E0158
RED BLOOD CELLS CPD/450mL/refg Plasma added	E0166
RED BLOOD CELLS CPD/450mL/refg ResLeu:<1log6 Plts/Cryo reduced	E3937
RED BLOOD CELLS CPD/450mL/refg ResLeu:<5log6	E0164
RED BLOOD CELLS CPD/450mL/refg Irradiated ResLeu:<1log6 Plasma reduced	E3936
RED BLOOD CELLS CPD/500mL/refg	E0167
RED BLOOD CELLS CPD/500mL/refg For mnf:injectable	E0168
RED BLOOD CELLS CPD/500mL/refg For mnf:noninjectable	E0169
RED BLOOD CELLS CPD/500mL/refg Irradiated	E0178
RED BLOOD CELLS CPD/500mL/refg Irradiated Plasma added	E0180
RED BLOOD CELLS CPD/500mL/refg Irradiated ResLeu:<5log6	E0179
RED BLOOD CELLS CPD/500mL/refg Not for tx or mnf.....	E0170
RED BLOOD CELLS CPD/500mL/refg Open	E0171
RED BLOOD CELLS CPD/500mL/refg Open Albumin added	E0176
RED BLOOD CELLS CPD/500mL/refg Open Irradiated	E0172
RED BLOOD CELLS CPD/500mL/refg Open Irradiated Plasma added	E0174
RED BLOOD CELLS CPD/500mL/refg Open Irradiated ResLeu:<5log6	E0173
RED BLOOD CELLS CPD/500mL/refg Open Plasma added	E0177
RED BLOOD CELLS CPD/500mL/refg Open ResLeu:<5log6	E0175
RED BLOOD CELLS CPD/500mL/refg Plasma added	E0183
RED BLOOD CELLS CPD/500mL/refg ResLeu:<5log6	E0181
RED BLOOD CELLS CPD/XX/refg	E0191
RED BLOOD CELLS CPD/XX/refg For mnf:injectable	E0192
RED BLOOD CELLS CPD/XX/refg For mnf:noninjectable.....	E0193
RED BLOOD CELLS CPD/XX/refg Not for tx or mnf.....	E0194

<u>Product Description</u>	<u>Product Code</u>
RED BLOOD CELLS CPDA-1/250mL/refg.....	E0229
RED BLOOD CELLS CPDA-1/250mL/refg For mnf:injectable.....	E0230
RED BLOOD CELLS CPDA-1/250mL/refg For mnf:noninjectable.....	E0231
RED BLOOD CELLS CPDA-1/250mL/refg Irradiated.....	E0237
RED BLOOD CELLS CPDA-1/250mL/refg Irradiated ResLeu:<5log6	E0238
RED BLOOD CELLS CPDA-1/250mL/refg Not for tx or mnf	E0232
RED BLOOD CELLS CPDA-1/250mL/refg Open	E0233
RED BLOOD CELLS CPDA-1/250mL/refg Open Irradiated	E0234
RED BLOOD CELLS CPDA-1/250mL/refg Open Irradiated ResLeu:<5log6	E0235
RED BLOOD CELLS CPDA-1/250mL/refg Open ResLeu:<5log6	E0236
RED BLOOD CELLS CPDA-1/250mL/refg ResLeu:<5log6	E0239
RED BLOOD CELLS CPDA-1/450mL/refg	E0195
RED BLOOD CELLS CPDA-1/450mL/refg For mnf:injectable	E0196
RED BLOOD CELLS CPDA-1/450mL/refg For mnf:noninjectable	E0197
RED BLOOD CELLS CPDA-1/450mL/refg Irradiated.....	E0206
RED BLOOD CELLS CPDA-1/450mL/refg Irradiated Plasma added	E0208
RED BLOOD CELLS CPDA-1/450mL/refg Irradiated Plasma reduced	E3837
RED BLOOD CELLS CPDA-1/450mL/refg Irradiated ResLeu:<5log6	E0207
RED BLOOD CELLS CPDA-1/450mL/refg Not for tx or mnf	E0198
RED BLOOD CELLS CPDA-1/450mL/refg Open	E0199
RED BLOOD CELLS CPDA-1/450mL/refg Open Albumin added.....	E0204
RED BLOOD CELLS CPDA-1/450mL/refg Open Irradiated	E0200
RED BLOOD CELLS CPDA-1/450mL/refg Open Irradiated Plasma added	E0202
RED BLOOD CELLS CPDA-1/450mL/refg Open Irradiated ResLeu:<5log6	E0201
RED BLOOD CELLS CPDA-1/450mL/refg Open Plasma added	E0205
RED BLOOD CELLS CPDA-1/450mL/refg Open ResLeu:<5log6	E0203
RED BLOOD CELLS CPDA-1/450mL/refg Plasma added	E0211
RED BLOOD CELLS CPDA-1/450mL/refg Plasma reduced	E3823
RED BLOOD CELLS CPDA-1/450mL/refg ResLeu:<5log6	E0209
RED BLOOD CELLS CPDA-1/500mL/refg	E0212

<u>Product Description</u>	<u>Product Code</u>
RED BLOOD CELLS CPDA-1/500mL/refg For mnf:injectable.....	E0213
RED BLOOD CELLS CPDA-1/500mL/refg For mnf:noninjectable	E0214
RED BLOOD CELLS CPDA-1/500mL/refg Irradiated.....	E0223
RED BLOOD CELLS CPDA-1/500mL/refg Irradiated Plasma added	E0225
RED BLOOD CELLS CPDA-1/500mL/refg Irradiated ResLeu:<5log6	E0224
RED BLOOD CELLS CPDA-1/500mL/refg Not for tx or mnf	E0215
RED BLOOD CELLS CPDA-1/500mL/refg Open	E0216
RED BLOOD CELLS CPDA-1/500mL/refg Open Albumin added.....	E0221
RED BLOOD CELLS CPDA-1/500mL/refg Open Irradiated	E0217
RED BLOOD CELLS CPDA-1/500mL/refg Open Irradiated Plasma added	E0219
RED BLOOD CELLS CPDA-1/500mL/refg Open Irradiated ResLeu:<5log6	E0218
RED BLOOD CELLS CPDA-1/500mL/refg Open Plasma added	E0222
RED BLOOD CELLS CPDA-1/500mL/refg Open ResLeu:<5log6	E0220
RED BLOOD CELLS CPDA-1/500mL/refg Plasma added	E0228
RED BLOOD CELLS CPDA-1/500mL/refg ResLeu:<5log6	E0226
RED BLOOD CELLS CPDA-1/XX/refg	E0240
RED BLOOD CELLS CPDA-1/XX/refg For mnf:injectable	E0241
RED BLOOD CELLS CPDA-1/XX/refg For mnf:noninjectable	E0242
RED BLOOD CELLS CPDA-1/XX/refg Low volume.....	E0244
RED BLOOD CELLS CPDA-1/XX/refg Not for tx or mnf	E0243
Rejuvenated RED BLOOD CELLS None/250mL/refg	E0599
Rejuvenated RED BLOOD CELLS None/250mL/refg Irradiated	E0604
Rejuvenated RED BLOOD CELLS None/250mL/refg Not for tx or mnf.....	E0600
Rejuvenated RED BLOOD CELLS None/250mL/refg Not for tx or mnf Open	E0601
Rejuvenated RED BLOOD CELLS None/250mL/refg Open	E0602
Rejuvenated RED BLOOD CELLS None/250mL/refg Open Irradiated	E0603
Rejuvenated RED BLOOD CELLS None/450mL/refg	E0571
Rejuvenated RED BLOOD CELLS None/450mL/refg Albumin added	E0581
Rejuvenated RED BLOOD CELLS None/450mL/refg Irradiated	E0580
Rejuvenated RED BLOOD CELLS None/450mL/refg Not for tx or mnf.....	E0572

<u>Product Description</u>	<u>Product Code</u>
Rejuvenated RED BLOOD CELLS None/450mL/refg Not for tx or mnf Open	E0573
Rejuvenated RED BLOOD CELLS None/450mL/refg Open	E0574
Rejuvenated RED BLOOD CELLS None/450mL/refg Open Albumin added	E0576
Rejuvenated RED BLOOD CELLS None/450mL/refg Open Irradiated	E0575
Rejuvenated RED BLOOD CELLS None/450mL/refg Open Plasma added	E0577
Rejuvenated RED BLOOD CELLS None/450mL/refg Open Supernat rem	E0578
Rejuvenated RED BLOOD CELLS None/450mL/refg Open Supernat rem/Plasma added.....	E0579
Rejuvenated RED BLOOD CELLS None/450mL/refg Plasma added	E0582
Rejuvenated RED BLOOD CELLS None/450mL/refg Supernat rem	E0583
Rejuvenated RED BLOOD CELLS None/450mL/refg Supernat rem/Plasma added	E0584
Rejuvenated RED BLOOD CELLS None/500mL/refg	E0585
Rejuvenated RED BLOOD CELLS None/500mL/refg Albumin added	E0595
Rejuvenated RED BLOOD CELLS None/500mL/refg Irradiated	E0594
Rejuvenated RED BLOOD CELLS None/500mL/refg Not for tx or mnf.....	E0586
Rejuvenated RED BLOOD CELLS None/500mL/refg Not for tx or mnf Open	E0587
Rejuvenated RED BLOOD CELLS None/500mL/refg Open	E0588
Rejuvenated RED BLOOD CELLS None/500mL/refg Open Albumin added	E0590
Rejuvenated RED BLOOD CELLS None/500mL/refg Open Irradiated	E0589
Rejuvenated RED BLOOD CELLS None/500mL/refg Open Plasma added	E0591
Rejuvenated RED BLOOD CELLS None/500mL/refg Open Supernat rem	E0592
Rejuvenated RED BLOOD CELLS None/500mL/refg Open Supernat rem/Plasma added.....	E0593
Rejuvenated RED BLOOD CELLS None/500mL/refg Plasma added	E0596
Rejuvenated RED BLOOD CELLS None/500mL/refg Supernat rem	E0597
Rejuvenated RED BLOOD CELLS None/500mL/refg Supernat rem/Plasma added	E0598
SERUM None/XX/<=-18C	E3894
Thawed APHERESIS CRYOPRECIPITATE None/XX/rt	E3599
Thawed APHERESIS CRYOPRECIPITATE None/XX/rt Irradiated	E3600
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg	E1237
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg <200 mL	E1310
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg <200 mL Aphr not automated	E1311

Product Description

Product Code

Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg >=200 mL <400mL	E1314
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg >=200 mL <400mL Aphr not automated	E1315
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg >=400mL <600mL	E1318
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg >=600mL.....	E1320
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Aphr not automated	E1322
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Irradiated.....	E1286
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Irradiated <200 mL	E1291
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Irradiated <200 mL Aphr not automated	E1292
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Irradiated >=200 mL <400mL	E1295
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Irradiated >=200 mL <400mL Aphr not automated	E1296
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Irradiated >=400mL <600mL	E1299
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Irradiated >=600mL.....	E1301
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Irradiated Aphr not automated	E1303
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Not for tx or mnf	E1238
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Not for tx or mnf Aphr not automated.....	E1245
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Not for tx or mnf Open	E1239
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Not for tx or mnf Open Aphr not automated	E1242
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open	E1246
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open <200 mL.....	E1271
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open <200 mL Aphr not automated	E1272
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open >=200 mL <400mL.....	E1275
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open >=200 mL <400mL Aphr not automated	E1276
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open >=400mL <600mL	E1279
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open >=600mL.....	E1281
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open Aphr not automated	E1283
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open Irradiated.....	E1247
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open Irradiated <200 mL.....	E1252

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open Irradiated <200 mL Aphr not automated	E1253
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open Irradiated >=200 mL <400mL	E1256
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open Irradiated >=200 mL <400mL Aphr not automated	E1257
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open Irradiated >=400mL <600mL	E1260
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open Irradiated >=600mL	E1262
Thawed APHERESIS FRESH FROZEN PLASMA ACD-A/XX/refg Open Irradiated Aphr not automated	E1264
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg	E1149
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg <200 mL	E1222
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg <200 mL Aphr not automated	E1223
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg >=200 mL <400mL	E1226
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg >=200 mL <400mL Aphr not automated	E1227
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg >=400mL <600mL	E1230
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg >=600mL	E1232
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Aphr not automated	E1234
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Irradiated	E1198
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Irradiated <200 mL	E1203
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Irradiated <200 mL Aphr not automated	E1204
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Irradiated >=200 mL <400mL	E1207
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Irradiated >=200 mL <400mL Aphr not automated	E1208
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Irradiated >=400mL <600mL	E1211
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Irradiated >=600mL	E1213
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Irradiated Aphr not automated	E1215
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Not for tx or mnf	E1150
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Not for tx or mnf Aphr not automated	E1157
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Not for tx or mnf Open	E1151
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Not for tx or mnf Open Aphr not automated	E1154

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open	E1158
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open <200 mL.....	E1183
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open <200 mL Aphr not automated	E1184
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open >=200 mL <400mL.....	E1187
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open >=200 mL <400mL Aphr not automated	E1188
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open >=400mL <600mL	E1191
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open >=600mL.....	E1193
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open Aphr not automated	E1195
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open Irradiated.....	E1159
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open Irradiated <200 mL.....	E1164
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open Irradiated <200 mL Aphr not automated	E1165
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open Irradiated >=200 mL <400mL.....	E1168
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open Irradiated >=200 mL <400mL Aphr not automated	E1169
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open Irradiated >=400mL <600mL	E1172
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open Irradiated >=600mL.....	E1174
Thawed APHERESIS FRESH FROZEN PLASMA ACD-B/XX/refg Open Irradiated Aphr not automated	E1176
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg	E1325
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg <200 mL	E1398
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg <200 mL Aphr not automated	E1399
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg >=200 mL <400mL	E1402
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg >=200 mL <400mL Aphr not automated	E1403
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg >=400mL <600mL	E1406
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg >=600mL	E1408
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Aphr not automated	E1410
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Irradiated	E1374
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Irradiated <200 mL	E1379
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Irradiated <200 mL Aphr not automated	E1380

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Irradiated >=200 mL <400mL	E1383
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Irradiated >=200 mL <400mL Aphr not automated	E1384
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Irradiated >=400mL <600mL	E1387
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Irradiated >=600mL	E1389
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Irradiated Aphr not automated	E1391
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Not for tx or mnf.....	E1326
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Not for tx or mnf Aphr not automated	E1333
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Not for tx or mnf Open	E1327
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Not for tx or mnf Open Aphr not automated	E1330
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open.....	E1334
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open <200 mL	E1359
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open <200 mL Aphr not automated	E1360
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open >=200 mL <400mL	E1363
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open >=200 mL <400mL Aphr not automated	E1364
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open >=400mL <600mL	E1367
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open >=600mL.....	E1369
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open Aphr not automated	E1371
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open Irradiated.....	E1335
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open Irradiated <200 mL	E1340
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open Irradiated <200 mL Aphr not automated	E1341
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open Irradiated >=200 mL <400mL	E1344
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open Irradiated >=200 mL <400mL Aphr not automated	E1345
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open Irradiated >=400mL <600mL	E1348
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open Irradiated >=600mL.....	E1350
Thawed APHERESIS FRESH FROZEN PLASMA NaCitrate/XX/refg Open Irradiated Aphr not automated	E1352
Thawed APHERESIS PLASMA ACD-A/XX/refg	E2121

Product Description

Product Code

Thawed APHERESIS PLASMA ACD-A/XX/refg <200 mL	E2260
Thawed APHERESIS PLASMA ACD-A/XX/refg <200 mL Aphr not automated.....	E2265
Thawed APHERESIS PLASMA ACD-A/XX/refg <200 mL Frozen <=24h	E2261
Thawed APHERESIS PLASMA ACD-A/XX/refg <200 mL Frozen <=24h Aphr not automated.....	E2262
Thawed APHERESIS PLASMA ACD-A/XX/refg <200 mL Frozen >24h.....	E2263
Thawed APHERESIS PLASMA ACD-A/XX/refg <200 mL Frozen >24h Aphr not automated.....	E2264
Thawed APHERESIS PLASMA ACD-A/XX/refg >=200 mL <400mL	E2266
Thawed APHERESIS PLASMA ACD-A/XX/refg >=200 mL <400mL Aphr not automated	E2271
Thawed APHERESIS PLASMA ACD-A/XX/refg >=200 mL <400mL Frozen <=24h	E2267
Thawed APHERESIS PLASMA ACD-A/XX/refg >=200 mL <400mL Frozen <=24h Aphr not automated.....	E2268
Thawed APHERESIS PLASMA ACD-A/XX/refg >=200 mL <400mL Frozen >24h.....	E2269
Thawed APHERESIS PLASMA ACD-A/XX/refg >=200 mL <400mL Frozen >24h Aphr not automated	E2270
Thawed APHERESIS PLASMA ACD-A/XX/refg >=400mL <600mL.....	E2272
Thawed APHERESIS PLASMA ACD-A/XX/refg >=400mL <600mL Aphr not automated	E2277
Thawed APHERESIS PLASMA ACD-A/XX/refg >=400mL <600mL Frozen <=24h	E2273
Thawed APHERESIS PLASMA ACD-A/XX/refg >=400mL <600mL Frozen <=24h Aphr not automated.....	E2274
Thawed APHERESIS PLASMA ACD-A/XX/refg >=400mL <600mL Frozen >24h.....	E2275
Thawed APHERESIS PLASMA ACD-A/XX/refg >=400mL <600mL Frozen >24h Aphr not automated	E2276
Thawed APHERESIS PLASMA ACD-A/XX/refg >=600mL	E2278
Thawed APHERESIS PLASMA ACD-A/XX/refg >=600mL Aphr not automated.....	E2283
Thawed APHERESIS PLASMA ACD-A/XX/refg >=600mL Frozen <=24h	E2279
Thawed APHERESIS PLASMA ACD-A/XX/refg >=600mL Frozen <=24h Aphr not automated	E2280
Thawed APHERESIS PLASMA ACD-A/XX/refg >=600mL Frozen >24h	E2281
Thawed APHERESIS PLASMA ACD-A/XX/refg >=600mL Frozen >24h Aphr not automated	E2282
Thawed APHERESIS PLASMA ACD-A/XX/refg Aphr not automated	E2288
Thawed APHERESIS PLASMA ACD-A/XX/refg Frozen <=24h	E2284
Thawed APHERESIS PLASMA ACD-A/XX/refg Frozen <=24h Aphr not automated	E2285
Thawed APHERESIS PLASMA ACD-A/XX/refg Frozen >24h	E2286
Thawed APHERESIS PLASMA ACD-A/XX/refg Frozen >24h Aphr not automated.....	E2287

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated	E2218
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated <200 mL	E2225
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated <200 mL Aphr not automated.....	E2230
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated <200 mL Frozen <=24h	E2226
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated <200 mL Frozen <=24h Aphr not automated.....	E2227
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated <200 mL Frozen >24h	E2228
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated <200 mL Frozen >24h Aphr not automated.....	E2229
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=200 mL <400mL.....	E2231
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=200 mL <400mL Aphr not automated	E2236
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=200 mL <400mL Frozen <=24h	E2232
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=200 mL <400mL Frozen <=24h Aphr not automated	E2233
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=200 mL <400mL Frozen >24h.....	E2234
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=200 mL <400mL Frozen >24h Aphr not automated	E2235
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=400mL <600mL.....	E2237
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=400mL <600mL Aphr not automated	E2242
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=400mL <600mL Frozen <=24h	E2238
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=400mL <600mL Frozen <=24h Aphr not automated	E2239
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=400mL <600mL Frozen >24h.....	E2240
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=400mL <600mL Frozen >24h Aphr not automated	E2241
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=600mL	E2243
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=600mL Aphr not automated	E2248
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=600mL Frozen <=24h	E2244
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=600mL Frozen <=24h Aphr not automated	E2245
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=600mL Frozen >24h	E2246
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated >=600mL Frozen >24h Aphr not automated.....	E2247
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated Aphr not automated	E2253
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated Frozen <=24h	E2249

<u>Product Description</u>	<u>Product Code</u>
----------------------------	---------------------

Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated Frozen <=24h Aphr not automated	E2250
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated Frozen >24h	E2251
Thawed APHERESIS PLASMA ACD-A/XX/refg Irradiated Frozen >24h Aphr not automated	E2252
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf	E2122
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf <200 mL	E2137
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf <200 mL Aphr not automated	E2138
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf >=200 mL <400mL	E2139
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf >=200 mL <400mL Aphr not automated.....	E2140
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf >=400mL <600mL	E2141
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf >=400mL <600mL Aphr not automated.....	E2142
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf >=600mL	E2143
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf >=600mL Aphr not automated	E2144
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Aphr not automated	E2145
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open.....	E2123
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open <200 mL	E2126
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open <200 mL Aphr not automated	E2127
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open >=200 mL <400mL	E2128
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open >=200 mL <400mL Aphr not automated	E2129
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open >=400mL <600mL	E2130
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open >=400mL <600mL Aphr not automated	E2131
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open >=600mL.....	E2132
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open >=600mL Aphr not automated	E2133
Thawed APHERESIS PLASMA ACD-A/XX/refg Not for tx or mnf Open Aphr not automated	E2134
Thawed APHERESIS PLASMA ACD-A/XX/refg Open	E2146
Thawed APHERESIS PLASMA ACD-A/XX/refg Open <200 mL	E2189
Thawed APHERESIS PLASMA ACD-A/XX/refg Open <200 mL Aphr not automated.....	E2194
Thawed APHERESIS PLASMA ACD-A/XX/refg Open <200 mL Frozen <=24h	E2190
Thawed APHERESIS PLASMA ACD-A/XX/refg Open <200 mL Frozen <=24h Aphr not automated	E2191

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS PLASMA ACD-A/XX/refg Open <200 mL Frozen >24h	E2192
Thawed APHERESIS PLASMA ACD-A/XX/refg Open <200 mL Frozen >24h Aphr not automated.....	E2193
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=200 mL <400mL	E2195
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=200 mL <400mL Aphr not automated.....	E2200
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=200 mL <400mL Frozen <=24h	E2196
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=200 mL <400mL Frozen <=24h Aphr not automated	E2197
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=200 mL <400mL Frozen >24h	E2198
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=200 mL <400mL Frozen >24h Aphr not automated	E2199
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=400mL <600mL.....	E2201
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=400mL <600mL Aphr not automated	E2206
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=400mL <600mL Frozen <=24h	E2202
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=400mL <600mL Frozen <=24h Aphr not automated	E2203
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=400mL <600mL Frozen >24h.....	E2204
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=400mL <600mL Frozen >24h Aphr not automated	E2205
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=600mL	E2207
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=600mL Aphr not automated	E2212
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=600mL Frozen <=24h	E2208
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=600mL Frozen <=24h Aphr not automated	E2209
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=600mL Frozen >24h	E2210
Thawed APHERESIS PLASMA ACD-A/XX/refg Open >=600mL Frozen >24h Aphr not automated	E2211
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Aphr not automated	E2217
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Frozen <=24h.....	E2213
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Frozen <=24h Aphr not automated	E2214
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Frozen >24h	E2215
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Frozen >24h Aphr not automated	E2216
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated	E2147
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated <200 mL	E2154
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated <200 mL Aphr not automated.....	E2159

<u>Product Description</u>	<u>Product Code</u>
----------------------------	---------------------

Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated <200 mL Frozen <=24h	E2155
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated <200 mL Frozen <=24h Aphr not automated	E2156
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated <200 mL Frozen >24h	E2157
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated <200 mL Frozen >24h Aphr not automated	E2158
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=200 mL <400mL	E2160
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=200 mL <400mL Aphr not automated.....	E2165
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=200 mL <400mL Frozen <=24h	E2161
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=200 mL <400mL Frozen <=24h Aphr	E2162
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=200 mL <400mL Frozen >24h	E2163
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=200 mL <400mL Frozen >24h Aphr not automated	E2164
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=400mL <600mL.....	E2166
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=400mL <600mL Aphr not automated	E2171
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=400mL <600mL Frozen <=24h	E2167
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=400mL <600mL Frozen <=24h Aphr	E2168
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=400mL <600mL Frozen >24h	E2169
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=400mL <600mL Frozen >24h Aphr not automated	E2170
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=600mL	E2172
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=600mL Aphr not automated	E2177
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=600mL Frozen <=24h	E2173
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=600mL Frozen <=24h Aphr not automated	E2174
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=600mL Frozen >24h	E2175
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated >=600mL Frozen >24h Aphr not automated	E2176
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated Aphr not automated	E2182
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated Frozen <=24h.....	E2178
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated Frozen <=24h Aphr not automated	E2179
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated Frozen >24h	E2180

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS PLASMA ACD-A/XX/refg Open Irradiated Frozen >24h Aphr not automated	E2181
Thawed APHERESIS PLASMA ACD-B/XX/refg	E1953
Thawed APHERESIS PLASMA ACD-B/XX/refg <200 mL	E2092
Thawed APHERESIS PLASMA ACD-B/XX/refg <200 mL Aphr not automated.....	E2097
Thawed APHERESIS PLASMA ACD-B/XX/refg <200 mL Frozen <=24h	E2093
Thawed APHERESIS PLASMA ACD-B/XX/refg <200 mL Frozen <=24h Aphr not automated.....	E2094
Thawed APHERESIS PLASMA ACD-B/XX/refg <200 mL Frozen >24h	E2095
Thawed APHERESIS PLASMA ACD-B/XX/refg <200 mL Frozen >24h Aphr not automated.....	E2096
Thawed APHERESIS PLASMA ACD-B/XX/refg >=200 mL <400mL	E2098
Thawed APHERESIS PLASMA ACD-B/XX/refg >=200 mL <400mL Aphr not automated	E2103
Thawed APHERESIS PLASMA ACD-B/XX/refg >=200 mL <400mL Frozen <=24h	E2099
Thawed APHERESIS PLASMA ACD-B/XX/refg >=200 mL <400mL Frozen <=24h Aphr not automated.....	E2100
Thawed APHERESIS PLASMA ACD-B/XX/refg >=200 mL <400mL Frozen >24h.....	E2101
Thawed APHERESIS PLASMA ACD-B/XX/refg >=200 mL <400mL Frozen >24h Aphr not automated	E2102
Thawed APHERESIS PLASMA ACD-B/XX/refg >=400mL <600mL.....	E2104
Thawed APHERESIS PLASMA ACD-B/XX/refg >=400mL <600mL Aphr not automated	E2109
Thawed APHERESIS PLASMA ACD-B/XX/refg >=400mL <600mL Frozen <=24h.....	E2105
Thawed APHERESIS PLASMA ACD-B/XX/refg >=400mL <600mL Frozen <=24h Aphr not automated.....	E2106
Thawed APHERESIS PLASMA ACD-B/XX/refg >=400mL <600mL Frozen >24h.....	E2107
Thawed APHERESIS PLASMA ACD-B/XX/refg >=400mL <600mL Frozen >24h Aphr not automated	E2108
Thawed APHERESIS PLASMA ACD-B/XX/refg >=600mL	E2110
Thawed APHERESIS PLASMA ACD-B/XX/refg >=600mL Aphr not automated	E2115
Thawed APHERESIS PLASMA ACD-B/XX/refg >=600mL Frozen <=24h	E2111
Thawed APHERESIS PLASMA ACD-B/XX/refg >=600mL Frozen <=24h Aphr not automated	E2112
Thawed APHERESIS PLASMA ACD-B/XX/refg >=600mL Frozen >24h	E2113
Thawed APHERESIS PLASMA ACD-B/XX/refg >=600mL Frozen >24h Aphr not automated.....	E2114
Thawed APHERESIS PLASMA ACD-B/XX/refg Aphr not automated	E2120
Thawed APHERESIS PLASMA ACD-B/XX/refg Frozen <=24h	E2116
Thawed APHERESIS PLASMA ACD-B/XX/refg Frozen <=24h Aphr not automated	E2117

<u>Product Description</u>	<u>Product Code</u>
-----------------------------------	----------------------------

Thawed APHERESIS PLASMA ACD-B/XX/refg Frozen >24h	E2118
Thawed APHERESIS PLASMA ACD-B/XX/refg Frozen >24h Aphr not automated.....	E2119
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated	E2050
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated <200 mL	E2057
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated <200 mL Aphr not automated.....	E2062
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated <200 mL Frozen <=24h	E2058
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated <200 mL Frozen <=24h Aphr not automated.....	E2059
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated <200 mL Frozen >24h	E2060
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated <200 mL Frozen >24h Aphr not automated.....	E2061
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=200 mL <400mL.....	E2063
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=200 mL <400mL Aphr not automated	E2068
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=200 mL <400mL Frozen <=24h	E2064
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=200 mL <400mL Frozen <=24h Aphr not automated	E2065
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=200 mL <400mL Frozen >24h.....	E2066
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=200 mL <400mL Frozen >24h Aphr not automated	E2067
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=400mL <600mL.....	E2069
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=400mL <600mL Aphr not automated	E2074
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=400mL <600mL Frozen <=24h	E2070
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=400mL <600mL Frozen <=24h Aphr not automated	E2071
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=400mL <600mL Frozen >24h.....	E2072
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=400mL <600mL Frozen >24h Aphr not automated	E2073
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=600mL	E2075
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=600mL Aphr not automated	E2080
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=600mL Frozen <=24h	E2076
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=600mL Frozen <=24h Aphr not automated	E2077
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=600mL Frozen >24h	E2078
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated >=600mL Frozen >24h Aphr not automated.....	E2079

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated Aphr not automated	E2085
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated Frozen <=24h	E2081
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated Frozen <=24h Aphr not automated	E2082
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated Frozen >24h	E2083
Thawed APHERESIS PLASMA ACD-B/XX/refg Irradiated Frozen >24h Aphr not automated	E2084
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf	E1954
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf <200 mL	E1969
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf <200 mL Aphr not automated	E1970
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf >=200 mL <400mL	E1971
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf >=200 mL <400mL Aphr not automated.....	E1972
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf >=400mL <600mL	E1973
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf >=400mL <600mL Aphr not automated.....	E1974
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf >=600mL	E1975
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf >=600mL Aphr not automated	E1976
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Aphr not automated	E1977
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open.....	E1955
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open <200 mL	E1958
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open <200 mL Aphr not automated	E1959
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open >=200 mL <400mL	E1960
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open >=200 mL <400mL Aphr not	E1961 automated
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open >=400mL <600mL	E1962
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open >=400mL <600mL Aphr not	E1963 automated
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open >=600mL.....	E1964
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open >=600mL Aphr not automated	E1965
Thawed APHERESIS PLASMA ACD-B/XX/refg Not for tx or mnf Open Aphr not automated	E1966
Thawed APHERESIS PLASMA ACD-B/XX/refg Open	E1978
Thawed APHERESIS PLASMA ACD-B/XX/refg Open <200 mL	E2021
Thawed APHERESIS PLASMA ACD-B/XX/refg Open <200 mL Aphr not automated.....	E2026

Product Description **Product Code**

Thawed APHERESIS PLASMA ACD-B/XX/refg Open <200 mL Frozen <=24h	E2022
Thawed APHERESIS PLASMA ACD-B/XX/refg Open <200 mL Frozen <=24h Aphr not automated	E2023
Thawed APHERESIS PLASMA ACD-B/XX/refg Open <200 mL Frozen >24h	E2024
Thawed APHERESIS PLASMA ACD-B/XX/refg Open <200 mL Frozen >24h Aphr not automated.....	E2025
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=200 mL <400mL	E2027
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=200 mL <400mL Aphr not automated.....	E2032
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=200 mL <400mL Frozen <=24h	E2028
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=200 mL <400mL Frozen <=24h Aphr not automated	E2029
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=200 mL <400mL Frozen >24h	E2030
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=200 mL <400mL Frozen >24h Aphr not automated	E2031
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=400mL <600mL.....	E2033
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=400mL <600mL Aphr not automated	E2038
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=400mL <600mL Frozen <=24h	E2034
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=400mL <600mL Frozen <=24h Aphr not automated	E2035
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=400mL <600mL Frozen >24h.....	E2036
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=400mL <600mL Frozen >24h Aphr not automated	E2037
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=600mL	E2039
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=600mL Aphr not automated	E2044
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=600mL Frozen <=24h	E2040
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=600mL Frozen <=24h Aphr not automated	E2041
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=600mL Frozen >24h	E2042
Thawed APHERESIS PLASMA ACD-B/XX/refg Open >=600mL Frozen >24h Aphr not automated.....	E2043
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Aphr not automated	E2049
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Frozen <=24h.....	E2045
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Frozen <=24h Aphr not automated	E2046
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Frozen >24h	E2047
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Frozen >24h Aphr not automated	E2048
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated	E1979

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated <200 mL	E1986
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated <200 mL Aphr not automated.....	E1991
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated <200 mL Frozen <=24h	E1987
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated <200 mL Frozen <=24h Aphr not automated	E1988
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated <200 mL Frozen >24h	E1989
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated <200 mL Frozen >24h Aphr not automated	E1990
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=00mL Frozen >24h Aphr not automated	E2008
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=200 mL <400mL	E1992
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=200 mL <400mL Aphr not automated.....	E1997
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=200 mL <400mL Frozen <=24h	E1993
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=200 mL <400mL Frozen <=24h Aphr not automated	E1994
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=200 mL <400mL Frozen >24h	E1995
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=200 mL <400mL Frozen >24h Aphr not automated	E1996
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=400mL <600mL	E1998
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=400mL <600mL Aphr not automated	E2003
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=400mL <600mL Frozen <=24h	E1999
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=400mL <600mL Frozen <=24h Aphr not automated	E2000
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=400mL <600mL Frozen >24h	E2001
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=400mL <600mL Frozen >24h Aphr not automated	E2002
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=600mL	E2004
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=600mL Aphr not automated	E2009
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=600mL Frozen <=24h	E2005
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=600mL Frozen <=24h Aphr not automated	E2006
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated >=600mL Frozen >24h	E2007
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated Aphr not automated	E2014
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated Frozen <=24h.....	E2010

Product Description

Product Code

Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated Frozen <=24h Aphr not automated	E2011
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated Frozen >24h	E2012
Thawed APHERESIS PLASMA ACD-B/XX/refg Open Irradiated Frozen >24h Aphr not automated	E2013
Thawed APHERESIS PLASMA NaCitrate/XX/refg	E2289
Thawed APHERESIS PLASMA NaCitrate/XX/refg <200 mL.....	E2428
Thawed APHERESIS PLASMA NaCitrate/XX/refg <200 mL Aphr not automated	E2433
Thawed APHERESIS PLASMA NaCitrate/XX/refg <200 mL Frozen <=24h.....	E2429
Thawed APHERESIS PLASMA NaCitrate/XX/refg <200 mL Frozen <=24h Aphr not automated.....	E2430
Thawed APHERESIS PLASMA NaCitrate/XX/refg <200 mL Frozen >24h.....	E2431
Thawed APHERESIS PLASMA NaCitrate/XX/refg <200 mL Frozen >24h Aphr not automated	E2432
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=200 mL <400mL.....	E2434
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=200 mL <400mL Aphr not automated	E2439
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=200 mL <400mL Frozen <=24h.....	E2435
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=200 mL <400mL Frozen <=24h Aphr not automated	E2436
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=200 mL <400mL Frozen >24h.....	E2437
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=200 mL <400mL Frozen >24h Aphr not automated	E2438
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=200 mL <600mL	E2440
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=400mL <600mL Aphr not automated	E2445
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=400mL <600mL Frozen <=24h	E2441
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=400mL <600mL Frozen <=24h Aphr not automated	E2442
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=400mL <600mL Frozen >24h	E2443
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=400mL <600mL Frozen >24h Aphr not automated	E2444
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=600mL	E2446
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=600mL Aphr not automated.....	E2451
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=600mL Frozen <=24h	E2447
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=600mL Frozen <=24h Aphr not automated	E2448
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=600mL Frozen >24h.....	E2449
Thawed APHERESIS PLASMA NaCitrate/XX/refg >=600mL Frozen >24h Aphr not automated	E2450

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS PLASMA NaCitrate/XX/refg Aphr not automated.....	E2456
Thawed APHERESIS PLASMA NaCitrate/XX/refg Frozen <=24h	E2452
Thawed APHERESIS PLASMA NaCitrate/XX/refg Frozen <=24h Aphr not automated.....	E2453
Thawed APHERESIS PLASMA NaCitrate/XX/refg Frozen >24h	E2454
Thawed APHERESIS PLASMA NaCitrate/XX/refg Frozen >24h Aphr not automated	E2455
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated	E2386
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated <200 mL.....	E2393
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated <200 mL Aphr not automated	E2398
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated <200 mL Frozen <=24h	E2394
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated <200 mL Frozen <=24h Aphr not automated.....	E2395
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated <200 mL Frozen >24h.....	E2396
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated <200 mL Frozen >24h Aphr not automated	E2397
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=200 mL <400mL.....	E2399
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=200 mL <400mL Aphr not automated	E2404
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=200 mL <400mL Frozen <=24h.....	E2400
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=200 mL <400mL Frozen <=24h Aphr not automated	E2401
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=200 mL <400mL Frozen >24h.....	E2402
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=200 mL <400mL Frozen >24h Aphr not automated	E2403
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=400mL <600mL	E2405
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=400mL <600mL Aphr not automated	E2410
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=400mL <600mL Frozen <=24h.....	E2406
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=400mL <600mL Frozen <=24h Aphr not automated	E2407
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=400mL <600mL Frozen >24h	E2408
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=400mL <600mL Frozen >24h Aphr not automated	E2409
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=600mL	E2411
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=600mL Aphr not automated.....	E2416
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=600mL Frozen <=24h	E2412

<u>Product Description</u>	<u>Product Code</u>
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=600mL Frozen <=24h Aphr not automated..... E2413	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=600mL Frozen >24h..... E2414	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated >=600mL Frozen >24h Aphr not automated E2415	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated Aphr not automated..... E2421	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated Frozen <=24h E2417	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated Frozen <=24h Aphr not automated E2418	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated Frozen >24h E2419	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Irradiated Frozen >24h Aphr not automated E2420	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf E2290	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf <200 mL E2305	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf <200 mL Aphr not automated E2306	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf >=200 mL <400mL E2307	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf >=200 mL <400mL Aphr not automated E2308	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf >=400mL <600mL E2309	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf >=400mL <600mL Aphr not automated E2310	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf >=600mL E2311	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf >=600mL Aphr not automated E2312	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Aphr not automated E2313	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open E2291	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open <200 mL E2294	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open <200 mL Aphr not automated E2295	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open >=200 mL <400mL E2296	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open >=200 mL <400mL Aphr not automated E2297	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open >=400mL <600mL E2298	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open >=400mL <600mL Aphr not automated E2299	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open >=600mL E2300	
Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open >=600mL Aphr not automated E2301	

Product Description **Product Code**

Thawed APHERESIS PLASMA NaCitrate/XX/refg Not for tx or mnf Open Aphr not automated	E2302
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open	E2314
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open <200 mL	E2357
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open <200 mL Aphr not automated.....	E2362
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open <200 mL Frozen <=24h	E2358
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open <200 mL Frozen <=24h Aphr not automated.....	E2359
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open <200 mL Frozen >24h	E2360
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open <200 mL Frozen >24h Aphr not automated	E2361
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=200 mL <400mL.....	E2363
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=200 mL <400mL Aphr not automated	E2368
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=200 mL <400mL Frozen <=24h	E2364
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=200 mL <400mL Frozen <=24h Aphr not automated	E2365
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=200 mL <400mL Frozen >24h.....	E2366
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=200 mL <400mL Frozen >24h Aphr not automated	E2367
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=400mL <600mL.....	E2369
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=400mL <600mL Aphr not automated	E2374
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=400mL <600mL Frozen <=24h	E2370
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=400mL <600mL Frozen <=24h Aphr not automated	E2371
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=400mL <600mL Frozen >24h.....	E2372
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=400mL <600mL Frozen >24h Aphr not automated	E2373
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=600mL	E2375
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=600mL Aphr not automated.....	E2380
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=600mL Frozen <=24h	E2376
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=600mL Frozen <=24h Aphr not automated	E2377
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=600mL Frozen >24h	E2378
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open >=600mL Frozen >24h Aphr not automated.....	E2379
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Aphr not automated	E2385
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Frozen <=24h	E2381

Product Description **Product Code**

Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Frozen <=24h Aphr not automated	E2382
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Frozen >24h	E2383
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Frozen >24h Aphr not automated.....	E2384
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated	E2315
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated <200 mL	E2322
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated <200 mL Aphr not automated.....	E2327
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated <200 mL Frozen <=24h	E2323
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated <200 mL Frozen <=24h Aphr not automated	E2324
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated <200 mL Frozen >24h	E2325
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated <200 mL Frozen >24h Aphr not automated	E2326
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=200 mL <400mL	E2328
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=200 mL <400mL Aphr not automated	E2333
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=200 mL <400mL Frozen <=24h	E2329
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=200 mL <400mL Frozen <=24h Aphr	E2330
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=200 mL <400mL Frozen >24h	E2331
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=200 mL <400mL Frozen >24h Aphr	E2332
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=400mL <600mL	E2334
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=400mL <600mL Aphr not automated	E2339
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=400mL <600mL Frozen <=24h	E2335
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=400mL <600mL Frozen <=24h Aphr	E2336
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=400mL <600mL Frozen >24h	E2337
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=400mL <600mL Frozen >24h Aphr	E2338
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=600mL	E2340
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=600mL Aphr not automated	E2345
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=600mL Frozen <=24h	E2341
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=600mL Frozen <=24h Aphr not automated	E2342

Product Description

Product Code

Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=600mL Frozen >24h	E2343
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated >=600mL Frozen >24h Aphr not automated	E2344
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated Aphr not automated	E2350
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated Frozen <=24h	E2346
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated Frozen <=24h Aphr not automated	E2347
Thawed APHERESIS PLASMA NaCitrate/XX/refg Open Irradiated Frozen >24h	E2348
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Not for tx or mnf Open	E3465
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Not for tx or mnf Open Plasma added	E3466
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open	E3467
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open 1st container	E3525
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open 1st container:not auto	E3529
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open 2nd container	E3526
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open 2nd container:not auto	E3530
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open 3rd container	E3527
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open 4th container	E3528
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Aphr not automated	E3524
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated	E3468
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated 1st container	E3494
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated 1st container:not auto	E3498
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated 2nd container	E3495
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated 2nd container:not auto	E3499
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated 3rd container	E3496
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated 4th container	E3497
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated Aphr not automated	E3493
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated Plasma added	E3485
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated Plasma added 1st container	E3487
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Irradiated Plasma added 1st container:not auto	E3491

Product Description

Product Code

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|Plasma added|2nd container..... E3488

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|Plasma added|2nd container:not auto E3492

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|Plasma added|3rd container E3489

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|Plasma added|4th container E3490

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|Plasma added|Aphr not automated..... E3486

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6 E3469

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|1st container..... E3479

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|1st container:not auto E3483

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|2nd container E3480

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|2nd container:not auto E3484

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|3rd container E3481

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|4th container..... E3482

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|Aphr not automated E3478

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|Plasma added..... E3470

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|Plasma added|1st container E3472

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|Plasma added|1st container:not auto E3476

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|Plasma added|2nd container E3473

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|Plasma added|2nd container:not auto E3477

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|Plasma added|3rd container E3474

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|Plasma added|4th container E3475

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Irradiated|ResLeu:<5log6|Plasma added|Aphr not automated E3471

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Plasma added E3516

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Plasma added|1st container E3518

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Plasma added|1st container:not auto E3522

Thawed APHERESIS PLATELETS|DMSO/XX/20-24C|Open|Plasma added|2nd container E3519

<u>Product Description</u>	<u>Product Code</u>
----------------------------	---------------------

Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Plasma added 2nd container:not auto	E3523
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Plasma added 3rd container	E3520
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Plasma added 4th container	E3521
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open Plasma added Aphr not automated.....	E3517
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6	E3500
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 1st container.....	E3510
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 1st container:not auto	E3514
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 2nd container	E3511
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 2nd container:not auto	E3515
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 3rd container	E3512
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 4th container.....	E3513
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Aphr not automated.....	E3509
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Plasma added	E3501
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Plasma added 1st container	E3503
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Plasma added 1st container:not auto	E3507
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Plasma added 2nd container	E3504
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Plasma added 2nd container:not auto	E3508
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Plasma added 3rd container	E3505
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Plasma added 4th container	E3506
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Plasma added Aphr not	E3502
Thawed APHERESIS PLATELETS DMSO/XX/20-24C Open ResLeu:<5log6 Plasma added Aphr not automated	E3502
Thawed CRYOPRECIPITATE None/450mL/rt	E3577
Thawed CRYOPRECIPITATE None/450mL/rt Irradiated	E3578
Thawed CRYOPRECIPITATE None/500mL/rt	E3579
Thawed CRYOPRECIPITATE None/500mL/rt Irradiated	E3580
Thawed CRYOPRECIPITATE None/XX/rt	E3581
Thawed CRYOPRECIPITATE None/XX/rt Irradiated	E3582
Thawed FRESH FROZEN PLASMA CP2D/XX/refg.....	E0797

<u>Product Description</u>	<u>Product Code</u>
Thawed FRESH FROZEN PLASMA CP2D/XX/refg Irradiated.....	E0806
Thawed FRESH FROZEN PLASMA CP2D/XX/refg Not for tx or mnf	E0798
Thawed FRESH FROZEN PLASMA CP2D/XX/refg Not for tx or mnf Open	E0799
Thawed FRESH FROZEN PLASMA CP2D/XX/refg Open.....	E0802
Thawed FRESH FROZEN PLASMA CP2D/XX/refg Open Irradiated.....	E0803
Thawed FRESH FROZEN PLASMA CPD/450mL/refg Irradiated Frozen <=6h.....	E3943
Thawed FRESH FROZEN PLASMA CPD/XX/refg	E0773
Thawed FRESH FROZEN PLASMA CPD/XX/refg Irradiated	E0782
Thawed FRESH FROZEN PLASMA CPD/XX/refg Not for tx or mnf	E0774
Thawed FRESH FROZEN PLASMA CPD/XX/refg Not for tx or mnf Open.....	E0775
Thawed FRESH FROZEN PLASMA CPD/XX/refg Open	E0778
Thawed FRESH FROZEN PLASMA CPD/XX/refg Open Irradiated	E0779
Thawed FRESH FROZEN PLASMA CPDA-1/XX/refg.....	E0785
Thawed FRESH FROZEN PLASMA CPDA-1/XX/refg Irradiated.....	E0794
Thawed FRESH FROZEN PLASMA CPDA-1/XX/refg Not for tx or mnf	E0786
Thawed FRESH FROZEN PLASMA CPDA-1/XX/refg Not for tx or mnf Open	E0787
Thawed FRESH FROZEN PLASMA CPDA-1/XX/refg Open.....	E0790
Thawed FRESH FROZEN PLASMA CPDA-1/XX/refg Open Irradiated	E0791
Thawed PLASMA CP2D/XX/refg	E2720
Thawed PLASMA CP2D/XX/refg Cryo reduced	E2736
Thawed PLASMA CP2D/XX/refg Frozen <=24h	E2737
Thawed PLASMA CP2D/XX/refg Irradiated	E2733
Thawed PLASMA CP2D/XX/refg Irradiated Cryo reduced	E2734
Thawed PLASMA CP2D/XX/refg Irradiated Frozen <=24h	E2735
Thawed PLASMA CP2D/XX/refg Not for tx or mnf	E2721
Thawed PLASMA CP2D/XX/refg Not for tx or mnf Cryo reduced	E2725
Thawed PLASMA CP2D/XX/refg Not for tx or mnf Frozen <=24h.....	E2726
Thawed PLASMA CP2D/XX/refg Not for tx or mnf Open.....	E2722
Thawed PLASMA CP2D/XX/refg Not for tx or mnf Open Cryo reduced	E2723
Thawed PLASMA CP2D/XX/refg Not for tx or mnf Open Frozen <=24h	E2724

Product Description

Product Code

Thawed PLASMA CP2D/XX/refg Open	E2727
Thawed PLASMA CP2D/XX/refg Open Cryo reduced	E2731
Thawed PLASMA CP2D/XX/refg Open Frozen <=24h	E2732
Thawed PLASMA CP2D/XX/refg Open Irradiated	E2728
Thawed PLASMA CP2D/XX/refg Open Irradiated Cryo reduced	E2729
Thawed PLASMA CP2D/XX/refg Open Irradiated Frozen <=24h	E2730
Thawed PLASMA CPD/450mL/<-25C//Frozen <=6h	E4011
Thawed PLASMA CPD/450mL/<-25C/Frozen <=6h	E4009
Thawed PLASMA CPD/450mL/<-25C/Irradiated/Frozen <=6h	E4010
Thawed PLASMA CPD/450mL/<-25C/Irradiated/ResLeu:<1log6/Frozen <=6h.....	E4012
Thawed PLASMA CPD/XX/refg	E2684
Thawed PLASMA CPD/XX/refg Cryo reduced	E2700
Thawed PLASMA CPD/XX/refg Frozen <=24h	E2701
Thawed PLASMA CPD/XX/refg Irradiated	E2697
Thawed PLASMA CPD/XX/refg Irradiated Cryo reduced	E2698
Thawed PLASMA CPD/XX/refg Irradiated Frozen <=24h	E2699
Thawed PLASMA CPD/XX/refg Not for tx or mnf	E2685
Thawed PLASMA CPD/XX/refg Not for tx or mnf Cryo reduced	E2689
Thawed PLASMA CPD/XX/refg Not for tx or mnf Frozen <=24h	E2690
Thawed PLASMA CPD/XX/refg Not for tx or mnf Open	E2686
Thawed PLASMA CPD/XX/refg Not for tx or mnf Open Cryo reduced	E2687
Thawed PLASMA CPD/XX/refg Not for tx or mnf Open Frozen <=24h	E2688
Thawed PLASMA CPD/XX/refg Open	E2691
Thawed PLASMA CPD/XX/refg Open Cryo reduced	E2695
Thawed PLASMA CPD/XX/refg Open Frozen <=24h	E2696
Thawed PLASMA CPD/XX/refg Open Irradiated	E2692
Thawed PLASMA CPD/XX/refg Open Irradiated Cryo reduced	E2693
Thawed PLASMA CPD/XX/refg Open Irradiated Frozen <=24h	E2694
Thawed PLASMA CPDA-1/XX/refg	E2702
Thawed PLASMA CPDA-1/XX/refg Cryo reduced	E2718

<u>Product Description</u>	<u>Product Code</u>
Thawed PLASMA CPDA-1/XX/refg Frozen <=24h	E2719
Thawed PLASMA CPDA-1/XX/refg Irradiated	E2715
Thawed PLASMA CPDA-1/XX/refg Irradiated Cryo reduced	E2716
Thawed PLASMA CPDA-1/XX/refg Irradiated Frozen <=24h	E2717
Thawed PLASMA CPDA-1/XX/refg Not for tx or mnf	E2703
Thawed PLASMA CPDA-1/XX/refg Not for tx or mnf Cryo reduced	E2707
Thawed PLASMA CPDA-1/XX/refg Not for tx or mnf Frozen <=24h.....	E2708
Thawed PLASMA CPDA-1/XX/refg Not for tx or mnf Open.....	E2704
Thawed PLASMA CPDA-1/XX/refg Not for tx or mnf Open Cryo reduced	E2705
Thawed PLASMA CPDA-1/XX/refg Not for tx or mnf Open Frozen <=24h.....	E2706
Thawed PLASMA CPDA-1/XX/refg Open	E2709
Thawed PLASMA CPDA-1/XX/refg Open Cryo reduced	E2713
Thawed PLASMA CPDA-1/XX/refg Open Frozen <=24h	E2714
Thawed PLASMA CPDA-1/XX/refg Open Irradiated	E2710
Thawed PLASMA CPDA-1/XX/refg Open Irradiated Cryo reduced	E2711
Thawed PLASMA CPDA-1/XX/refg Open Irradiated Frozen <=24h	E2712
Thawed POOLED CRYOPRECIPITATE None/XX/rt	E3591
Thawed POOLED CRYOPRECIPITATE None/XX/rt Irradiated	E3594
Thawed POOLED CRYOPRECIPITATE None/XX/rt Open.....	E3592
Thawed POOLED CRYOPRECIPITATE None/XX/rt Open Irradiated.....	E3593
Washed APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 120 log9 plts	E3970
Washed APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 180 log9 plts	E3969
Washed APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Approx 240 log9 plts	E3968
Washed APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Supernat	E3973
reduced Approx 120 log9 plts	
Washed APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Supernat	E3972
reduced Approx 180 log9 plts	
Washed APHERESIS PLATELETS ACD-A/XX/20-24C Irradiated ResLeu:<2log5 Supernat	E3971
reduced Approx 240 log9 plts	
Washed APHERESIS PLATELETS None/XX/20-24C Not for tx or mnf Open	E3531

<u>Product Description</u>	<u>Product Code</u>
Washed APHERESIS PLATELETS None/XX/20-24C Not for tx or mnf Open 1st container.....	E3533
Washed APHERESIS PLATELETS None/XX/20-24C Not for tx or mnf Open 1st container:not auto	E3537
Washed APHERESIS PLATELETS None/XX/20-24C Not for tx or mnf Open 2nd container.....	E3534
Washed APHERESIS PLATELETS None/XX/20-24C Not for tx or mnf Open 2nd container:not auto	E3538
Washed APHERESIS PLATELETS None/XX/20-24C Not for tx or mnf Open 3rd container	E3535
Washed APHERESIS PLATELETS None/XX/20-24C Not for tx or mnf Open 4th container	E3536
Washed APHERESIS PLATELETS None/XX/20-24C Not for tx or mnf Open Aphr not automated.....	E3532
Washed APHERESIS PLATELETS None/XX/20-24C Open	E3539
Washed APHERESIS PLATELETS None/XX/20-24C Open 1st container	E3565
Washed APHERESIS PLATELETS None/XX/20-24C Open 1st container:not auto	E3569
Washed APHERESIS PLATELETS None/XX/20-24C Open 2nd container	E3566
Washed APHERESIS PLATELETS None/XX/20-24C Open 2nd container:not auto	E3570
Washed APHERESIS PLATELETS None/XX/20-24C Open 3rd container	E3567
Washed APHERESIS PLATELETS None/XX/20-24C Open 4th container	E3568
Washed APHERESIS PLATELETS None/XX/20-24C Open Aphr not automated	E3564
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated.....	E3540
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated 1st container	E3550
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated 1st container:not auto	E3554
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated 2nd container	E3551
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated 2nd container:not auto	E3555
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated 3rd container	E3552
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated 4th container	E3553
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated Aphr not automated	E3549
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated ResLeu:<5log6	E3541
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated ResLeu:<5log6 1st container	E3543
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated ResLeu:<5log6 1st container:not auto	E3547
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated ResLeu:<5log6 2nd container	E3544
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated ResLeu:<5log6 2nd container:not auto	E3548
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated ResLeu:<5log6 3rd container.....	E3545

<u>Product Description</u>	<u>Product Code</u>
-----------------------------------	----------------------------

Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated ResLeu:<5log6 4th container	E3546
Washed APHERESIS PLATELETS None/XX/20-24C Open Irradiated ResLeu:<5log6 Aphr not automated	E3542
Washed APHERESIS PLATELETS None/XX/20-24C Open ResLeu:<5log6	E3556
Washed APHERESIS PLATELETS None/XX/20-24C Open ResLeu:<5log6 1st container	E3558
Washed APHERESIS PLATELETS None/XX/20-24C Open ResLeu:<5log6 1st container:not auto.....	E3562
Washed APHERESIS PLATELETS None/XX/20-24C Open ResLeu:<5log6 2nd container	E3559
Washed APHERESIS PLATELETS None/XX/20-24C Open ResLeu:<5log6 2nd container:not auto.....	E3563
Washed APHERESIS PLATELETS None/XX/20-24C Open ResLeu:<5log6 3rd container.....	E3560
Washed APHERESIS PLATELETS None/XX/20-24C Open ResLeu:<5log6 4th container	E3561
Washed APHERESIS PLATELETS None/XX/20-24C Open ResLeu:<5log6 Aphr not automated	E3557
Washed PLATELETS None/XX/20-24C Open	E2889
Washed PLATELETS None/XX/20-24C Open Irradiated	E2890
Washed PLATELETS None/XX/20-24C Open Irradiated ResLeu:<8.3log5	E2891
Washed PLATELETS None/XX/20-24C Open ResLeu:<8.3log5	E2894
Washed POOLED PLATELETS None/XX/20-24C Not for tx or mnf Open.....	E2917
Washed POOLED PLATELETS None/XX/20-24C Open	E2918
Washed POOLED PLATELETS None/XX/20-24C Open Irradiated	E2919
Washed POOLED PLATELETS None/XX/20-24C Open Irradiated ResLeu:<5log6	E2920
Washed POOLED PLATELETS None/XX/20-24C Open ResLeu:<5log6	E2921
Washed POOLED PLATELETS PASII/XX/20-24C ResLeu:<2log5 Buffy coat plts prep From 3 donors	E3995
Washed RED BLOOD CELLS None/250mL/refg For mnf:injectable Open	E0490
Washed RED BLOOD CELLS None/250mL/refg For mnf:noninjectable Open	E0491
Washed RED BLOOD CELLS None/250mL/refg Not for tx or mnf Open	E0492
Washed RED BLOOD CELLS None/250mL/refg Open	E0493
Washed RED BLOOD CELLS None/250mL/refg Open Albumin added.....	E0499
Washed RED BLOOD CELLS None/250mL/refg Open Irradiated	E0494
Washed RED BLOOD CELLS None/250mL/refg Open Irradiated Albumin added.....	E0496
Washed RED BLOOD CELLS None/250mL/refg Open Irradiated Plasma added.....	E0497
Washed RED BLOOD CELLS None/250mL/refg Open Irradiated ResLeu:<5log6.....	E0495

<u>Product Description</u>	<u>Product Code</u>
Washed RED BLOOD CELLS None/250mL/refg Open Plasma added.....	E0500
Washed RED BLOOD CELLS None/250mL/refg Open ResLeu:<5log6.....	E0498
Washed RED BLOOD CELLS None/450mL/refg For mnf:injectable Open	E0468
Washed RED BLOOD CELLS None/450mL/refg For mnf:noninjectable Open	E0469
Washed RED BLOOD CELLS None/450mL/refg Not for tx or mnf Open	E0470
Washed RED BLOOD CELLS None/450mL/refg Open	E0471
Washed RED BLOOD CELLS None/450mL/refg Open Albumin added.....	E0477
Washed RED BLOOD CELLS None/450mL/refg Open Irradiated	E0472
Washed RED BLOOD CELLS None/450mL/refg Open Irradiated Albumin added.....	E0474
Washed RED BLOOD CELLS None/450mL/refg Open Irradiated Plasma added.....	E0475
Washed RED BLOOD CELLS None/450mL/refg Open Irradiated ResLeu:<1log6.....	E3852
Washed RED BLOOD CELLS None/450mL/refg Open Irradiated ResLeu:<5log6.....	E0473
Washed RED BLOOD CELLS None/450mL/refg Open Plasma added.....	E0478
Washed RED BLOOD CELLS None/450mL/refg Open ResLeu:<1log6.....	E3851
Washed RED BLOOD CELLS None/450mL/refg Open ResLeu:<5log6.....	E0476
Washed RED BLOOD CELLS None/500mL/refg For mnf:injectable Open	E0479
Washed RED BLOOD CELLS None/500mL/refg For mnf:noninjectable Open	E0480
Washed RED BLOOD CELLS None/500mL/refg Not for tx or mnf Open	E0481
Washed RED BLOOD CELLS None/500mL/refg Open	E0482
Washed RED BLOOD CELLS None/500mL/refg Open Albumin added.....	E0488
Washed RED BLOOD CELLS None/500mL/refg Open Irradiated	E0483
Washed RED BLOOD CELLS None/500mL/refg Open Irradiated Albumin added.....	E0485
Washed RED BLOOD CELLS None/500mL/refg Open Irradiated Plasma added.....	E0486
Washed RED BLOOD CELLS None/500mL/refg Open Irradiated ResLeu:<5log6.....	E0484
Washed RED BLOOD CELLS None/500mL/refg Open Plasma added.....	E0489
Washed RED BLOOD CELLS None/500mL/refg Open ResLeu:<5log6.....	E0487
WHOLE BLOOD CP2D/450mL/refg	E0098
WHOLE BLOOD CP2D/450mL/refg Cryo reduced.....	E0109
WHOLE BLOOD CP2D/450mL/refg For mnf:injectable	E0099
WHOLE BLOOD CP2D/450mL/refg For mnf:noninjectable	E0100

<u>Product Description</u>	<u>Product Code</u>
WHOLE BLOOD CP2D/450mL/refg Irradiated	E0106
WHOLE BLOOD CP2D/450mL/refg Irradiated ResLeu:<5log6.....	E0107
WHOLE BLOOD CP2D/450mL/refg Not for tx or mnf	E0101
WHOLE BLOOD CP2D/450mL/refg Open	E0102
WHOLE BLOOD CP2D/450mL/refg Open Irradiated	E0103
WHOLE BLOOD CP2D/450mL/refg Open Irradiated ResLeu:<5log6.....	E0104
WHOLE BLOOD CP2D/450mL/refg Open ResLeu:<5log6.....	E0105
WHOLE BLOOD CP2D/450mL/refg Plts reduced	E0110
WHOLE BLOOD CP2D/450mL/refg Plts/Cryo reduced	E0111
WHOLE BLOOD CP2D/450mL/refg ResLeu:<5log6.....	E0108
WHOLE BLOOD CP2D/500mL/refg	E0112
WHOLE BLOOD CP2D/500mL/refg Cryo reduced.....	E0123
WHOLE BLOOD CP2D/500mL/refg For mnf:injectable	E0113
WHOLE BLOOD CP2D/500mL/refg For mnf:noninjectable	E0114
WHOLE BLOOD CP2D/500mL/refg Irradiated	E0120
WHOLE BLOOD CP2D/500mL/refg Irradiated ResLeu:<5log6.....	E0121
WHOLE BLOOD CP2D/500mL/refg Not for tx or mnf	E0115
WHOLE BLOOD CP2D/500mL/refg Open	E0116
WHOLE BLOOD CP2D/500mL/refg Open Irradiated	E0117
WHOLE BLOOD CP2D/500mL/refg Open Irradiated ResLeu:<5log6.....	E0118
WHOLE BLOOD CP2D/500mL/refg Open ResLeu:<5log6.....	E0119
WHOLE BLOOD CP2D/500mL/refg Plts reduced	E0124
WHOLE BLOOD CP2D/500mL/refg Plts/Cryo reduced	E0125
WHOLE BLOOD CP2D/500mL/refg ResLeu:<5log6.....	E0122
WHOLE BLOOD CP2D/XX/refg	E0126
WHOLE BLOOD CP2D/XX/refg For mnf:injectable	E0127
WHOLE BLOOD CP2D/XX/refg For mnf:noninjectable	E0128
WHOLE BLOOD CP2D/XX/refg Low volume	E0130
WHOLE BLOOD CP2D/XX/refg Not for tx or mnf	E0129
WHOLE BLOOD CPD/250mL/refg.....	E0037

<u>Product Description</u>	<u>Product Code</u>
WHOLE BLOOD CPD/250mL/refg For mnf:injectable.....	E0038
WHOLE BLOOD CPD/250mL/refg For mnf:noninjectable	E0039
WHOLE BLOOD CPD/250mL/refg Irradiated.....	E0045
WHOLE BLOOD CPD/250mL/refg Irradiated ResLeu:<5log6	E0046
WHOLE BLOOD CPD/250mL/refg Not for tx or mnf.....	E0040
WHOLE BLOOD CPD/250mL/refg Open.....	E0041
WHOLE BLOOD CPD/250mL/refg Open Irradiated.....	E0042
WHOLE BLOOD CPD/250mL/refg Open Irradiated ResLeu:<5log6	E0043
WHOLE BLOOD CPD/250mL/refg Open ResLeu:<5log6	E0044
WHOLE BLOOD CPD/250mL/refg ResLeu:<5log6	E0047
WHOLE BLOOD CPD/450mL/refg.....	E0009
WHOLE BLOOD CPD/450mL/refg Cryo reduced	E0020
WHOLE BLOOD CPD/450mL/refg For mnf:injectable.....	E0010
WHOLE BLOOD CPD/450mL/refg For mnf:noninjectable	E0011
WHOLE BLOOD CPD/450mL/refg Irradiated.....	E0017
WHOLE BLOOD CPD/450mL/refg Irradiated ResLeu:<5log6	E0018
WHOLE BLOOD CPD/450mL/refg Not for tx or mnf.....	E0012
WHOLE BLOOD CPD/450mL/refg Open.....	E0013
WHOLE BLOOD CPD/450mL/refg Open Irradiated.....	E0014
WHOLE BLOOD CPD/450mL/refg Open Irradiated ResLeu:<5log6	E0015
WHOLE BLOOD CPD/450mL/refg Open ResLeu:<5log6	E0016
WHOLE BLOOD CPD/450mL/refg Plts reduced.....	E0021
WHOLE BLOOD CPD/450mL/refg Plts/Cryo reduced.....	E0022
WHOLE BLOOD CPD/450mL/refg ResLeu:<5log6	E0019
WHOLE BLOOD CPD/500mL/refg.....	E0023
WHOLE BLOOD CPD/500mL/refg Cryo reduced	E0034
WHOLE BLOOD CPD/500mL/refg For mnf:injectable.....	E0024
WHOLE BLOOD CPD/500mL/refg For mnf:noninjectable	E0025
WHOLE BLOOD CPD/500mL/refg Irradiated.....	E0031
WHOLE BLOOD CPD/500mL/refg Irradiated ResLeu:<5log6	E0032

<u>Product Description</u>	<u>Product Code</u>
WHOLE BLOOD CPD/500mL/refg Not for tx or mnf.....	E0026
WHOLE BLOOD CPD/500mL/refg Open.....	E0027
WHOLE BLOOD CPD/500mL/refg Open Irradiated.....	E0028
WHOLE BLOOD CPD/500mL/refg Open Irradiated ResLeu:<5log6	E0029
WHOLE BLOOD CPD/500mL/refg Open ResLeu:<5log6	E0030
WHOLE BLOOD CPD/500mL/refg Plts reduced.....	E0035
WHOLE BLOOD CPD/500mL/refg Plts/Cryo reduced.....	E0036
WHOLE BLOOD CPD/500mL/refg ResLeu:<5log6	E0033
WHOLE BLOOD CPD/XX/refg.....	E0048
WHOLE BLOOD CPD/XX/refg For mnf:injectable	E0049
WHOLE BLOOD CPD/XX/refg For mnf:noninjectable	E0050
WHOLE BLOOD CPD/XX/refg Low volume.....	E0052
WHOLE BLOOD CPD/XX/refg Not for tx or mnf	E0051
WHOLE BLOOD CPDA-1/250mL/refg	E0082
WHOLE BLOOD CPDA-1/250mL/refg For mnf:injectable	E0083
WHOLE BLOOD CPDA-1/250mL/refg For mnf:noninjectable	E0084
WHOLE BLOOD CPDA-1/250mL/refg Irradiated	E0090
WHOLE BLOOD CPDA-1/250mL/refg Irradiated ResLeu:<5log6.....	E0091
WHOLE BLOOD CPDA-1/250mL/refg Not for tx or mnf	E0085
WHOLE BLOOD CPDA-1/250mL/refg Open	E0086
WHOLE BLOOD CPDA-1/250mL/refg Open Irradiated	E0087
WHOLE BLOOD CPDA-1/250mL/refg Open Irradiated ResLeu:<5log6	E0088
WHOLE BLOOD CPDA-1/250mL/refg Open ResLeu:<5log6	E0089
WHOLE BLOOD CPDA-1/250mL/refg ResLeu:<5log6.....	E0092
WHOLE BLOOD CPDA-1/450mL/refg	E0053
WHOLE BLOOD CPDA-1/450mL/refg Cryo reduced	E0064
WHOLE BLOOD CPDA-1/450mL/refg For mnf:injectable	E0054
WHOLE BLOOD CPDA-1/450mL/refg For mnf:noninjectable	E0055
WHOLE BLOOD CPDA-1/450mL/refg Irradiated	E0061
WHOLE BLOOD CPDA-1/450mL/refg Irradiated ResLeu:<5log6.....	E0062

<u>Product Description</u>	<u>Product Code</u>
WHOLE BLOOD CPDA-1/450mL/refg Not for tx or mnf	E0056
WHOLE BLOOD CPDA-1/450mL/refg Open	E0057
WHOLE BLOOD CPDA-1/450mL/refg Open Irradiated	E0058
WHOLE BLOOD CPDA-1/450mL/refg Open Irradiated ResLeu:<5log6	E0059
WHOLE BLOOD CPDA-1/450mL/refg Open ResLeu:<5log6	E0060
WHOLE BLOOD CPDA-1/450mL/refg Plts reduced	E0065
WHOLE BLOOD CPDA-1/450mL/refg Plts/Cryo reduced	E0066
WHOLE BLOOD CPDA-1/450mL/refg ResLeu:<5log6	E0063
WHOLE BLOOD CPDA-1/500mL/refg	E0068
WHOLE BLOOD CPDA-1/500mL/refg Cryo reduced	E0079
WHOLE BLOOD CPDA-1/500mL/refg For mnf:injectable	E0069
WHOLE BLOOD CPDA-1/500mL/refg For mnf:noninjectable	E0070
WHOLE BLOOD CPDA-1/500mL/refg Irradiated	E0076
WHOLE BLOOD CPDA-1/500mL/refg Irradiated ResLeu:<5log6	E0077
WHOLE BLOOD CPDA-1/500mL/refg Not for tx or mnf	E0071
WHOLE BLOOD CPDA-1/500mL/refg Open	E0072
WHOLE BLOOD CPDA-1/500mL/refg Open Irradiated	E0073
WHOLE BLOOD CPDA-1/500mL/refg Open Irradiated ResLeu:<5log6	E0074
WHOLE BLOOD CPDA-1/500mL/refg Open ResLeu:<5log6	E0075
WHOLE BLOOD CPDA-1/500mL/refg Plts reduced	E0080
WHOLE BLOOD CPDA-1/500mL/refg Plts/Cryo reduced	E0081
WHOLE BLOOD CPDA-1/500mL/refg ResLeu:<5log6	E0078
WHOLE BLOOD CPDA-1/XX/refg	E0093
WHOLE BLOOD CPDA-1/XX/refg For mnf:injectable	E0094
WHOLE BLOOD CPDA-1/XX/refg For mnf:noninjectable	E0095
WHOLE BLOOD CPDA-1/XX/refg Low volume	E0097
WHOLE BLOOD CPDA-1/XX/refg Not for tx or mnf	E0096
WHOLE BLOOD Heparin/450mL/refg	E0135
WHOLE BLOOD Heparin/450mL/refg Irradiated	E3842
WHOLE BLOOD Heparin/450mL/refg Not for tx or mnf	E0136

<u>Product Description</u>	<u>Product Code</u>
WHOLE BLOOD Heparin/500mL/refg.....	E0137
WHOLE BLOOD Heparin/500mL/refg Not for tx or mnf.....	E0138
WHOLE BLOOD None/450mL/refg For mnf:injectable	E0139
WHOLE BLOOD None/450mL/refg For mnf:noninjectable	E0140
WHOLE BLOOD None/450mL/refg Not for tx or mnf	E0141

Index

AABB, 3
abbreviation, 15
ABO/Rh Blood Groups
 structure, 10
anticoagulant/additive, 17
ARC, 3
associated division, 16
autologous/directed component, 19, 20, 21, 22
BLOOD COMPONENT, 12
BLOOD INVENTORY File (#65), 8
 changed fields, 8
BLOOD PRODUCT File (#66), 7
 changed fields, 7
 new fields, 7
can be requested, 18
CCB, 3
CMV Antibody Status Report, 34
Codabar, 3
Codabar Limitations, 9
Code 128, 3
Code 128 Character Set, 9
collection/prep hours, 17
Component Elements of ISBT 128 Barcodes, 9
contains red blood cells, 18
CORE CONDITIONS, 12
cost, 20
criteria for use, 21
Crossmatch/Transfusion Report, 34
Crossmatch/Transfusions by Specialty/Physician, 34
days left, 17
DEFINITIONS, 3
description, 19
Disposition – Not Transfused, 27
Disposition - Relocation, 34
DoD, 3
DOD code, 16
Donation Identification Number, 9
Edit Unit Disposition Fields, 33
Edit Unit Log-in, 33
Edit Unit-patient Fields, 33
equivalent product, 17
expiration date, 21
Expiration Date/time
 structure, 11
FDA, 3
Field Changes, 7
File Changes, 7
ICCBBA, 3
identifier, 16
INTRODUCTION, 1
IS ISBT128, 16
ISBT, 3
March 2001

ISBT 128, 3
ISBT 128 BARCODE CHARACTERISTICS FOR U.S. IMPLEMENTATION, 9
ISBT 128 Blood Product Description, 11
LAB DATA File (#63)
 changed fields, 8
Log-in regular (invoices), 25
lot number, 21
max age for pediatric use, 18
maximum infusion time, 19
maximum storage days, 17
modification criteria, 16
modification of, 16
modified before release, 18
modify to, 19
OTHER ATTRIBUTES, 12
Patient Blood Bank Record, 34
Patient specimen age allowed, 18
patient/product ABO, 16
patient/product requirement, 17
patient/product RH, 17
pediatric product, 18
Pediatric Unit Preparation, 30
Phenotyped Units Available, 34
pre-op tests to check, 22
Print Data Change Audit, 34
Print Units With Final Disposition, 34
product code, 16
Product Code
 structure, 10
REFERENCES, 5
registration number, 21
requisition instructions, 22
retype after preparation, 18
Select Units for Patients, 33
SETTING UP A NEW ENTRY IN THE BLOOD PRODUCT File (#66), 15
SOFTWARE CHANGES, 6
Special Testing
 structure, 11
specific gravity, 18
specimen, 22
SRS, 4
supplier, 20
supplier preference number, 20
supplier prefix number, 21
synonym, 19
tests to check, 21
Transfusion Data Report, 34
Transfusions by Treating Specialty/physician, 34
Unit ABO/Rh Confirmation, 33, 34
unit label non-standard, 21
Units Assigned/Components Requested, 34
VBECS, 4
VISTA, 4

volume, 17
WKLD code, 22