



# Servive Master Config 6-Blue 6-Violet 3-355UV 3-Red


Cytometer:	LSRII	User:	Administrator
Cytometer Name:	LSRII	Institution:	DVAMC
Serial Number:	H47100187	Software:	BD FACSDiva 6.1.1
Input Device:	Manual	Date:	6/14/2017 11:23:11 AM
Window Extension:	10.00		

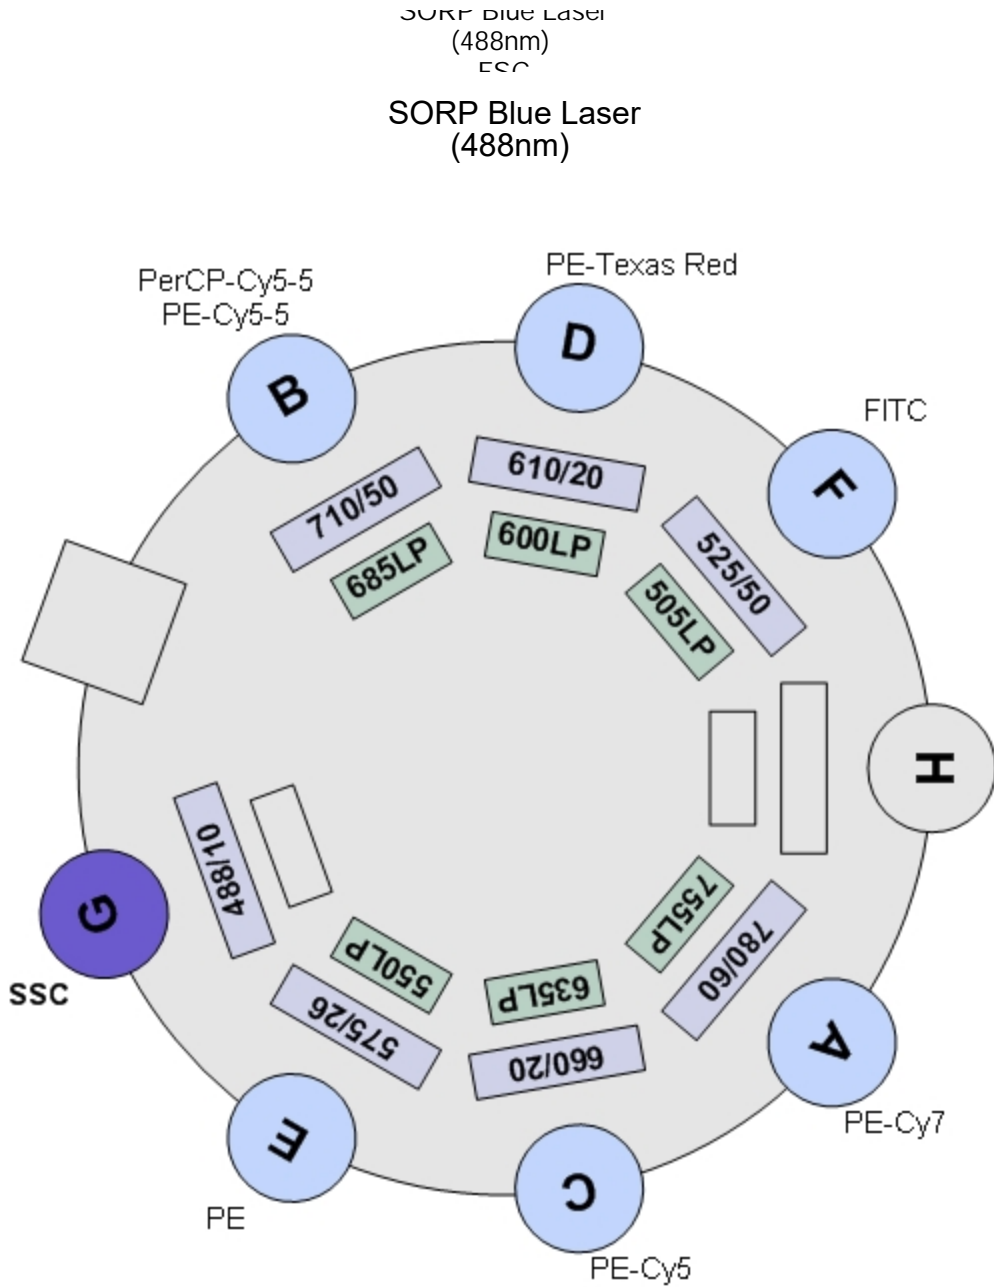


SORP Violet Laser  
(405nm)

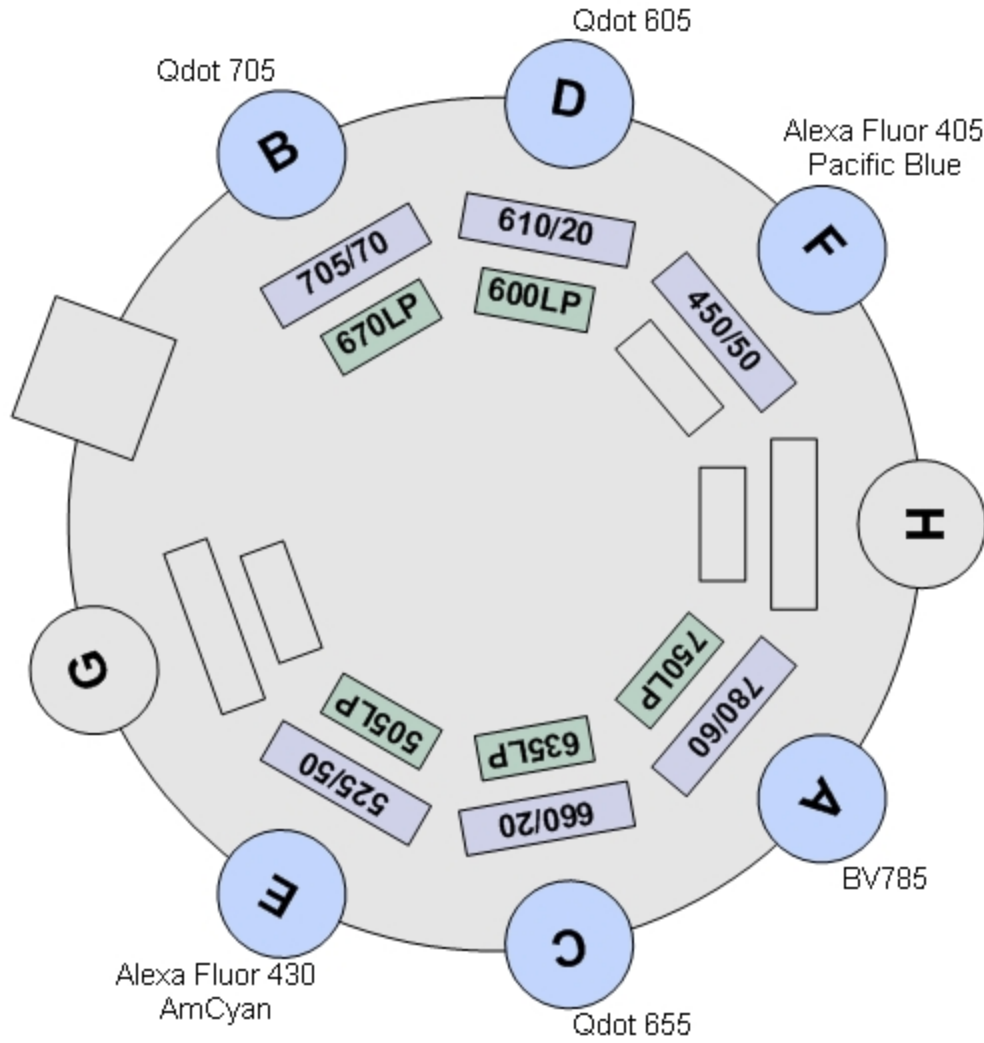

SORP UV Laser  
(355nm)

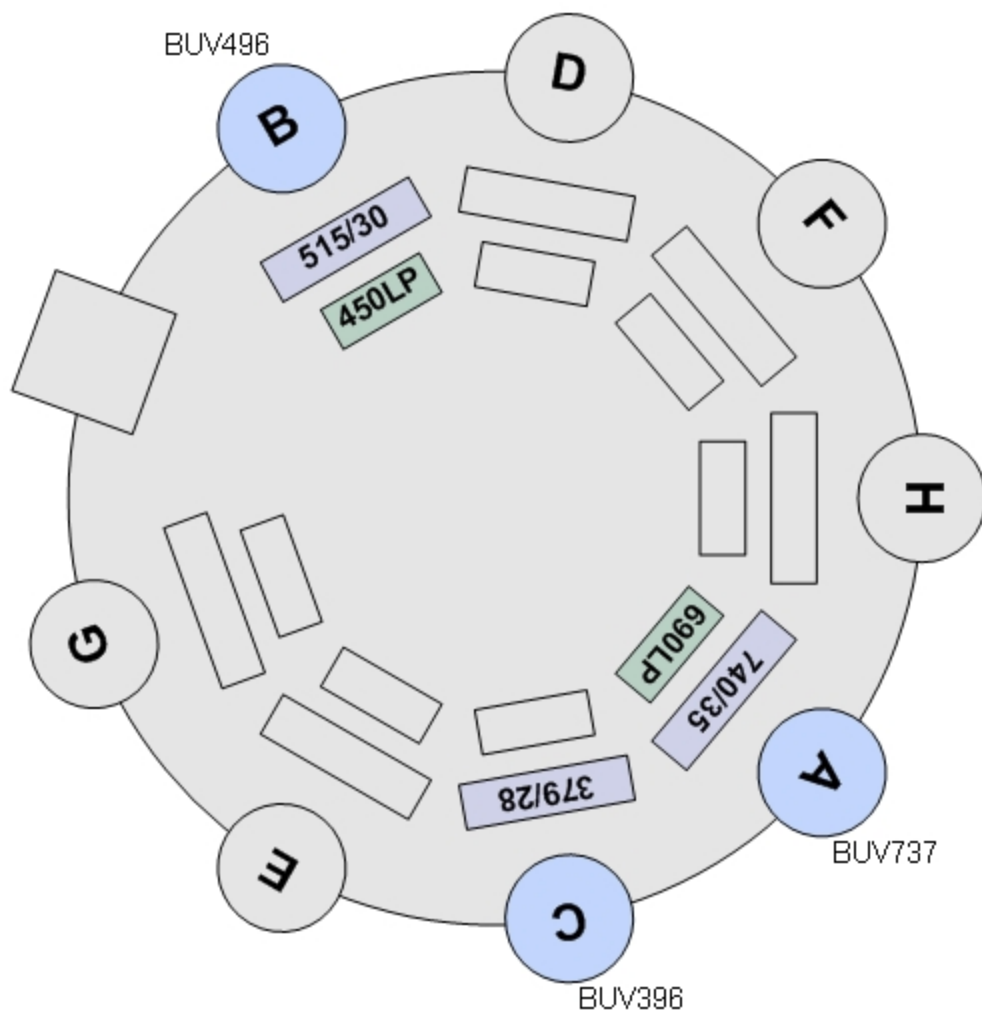

SORP Red Laser  
(640nm)

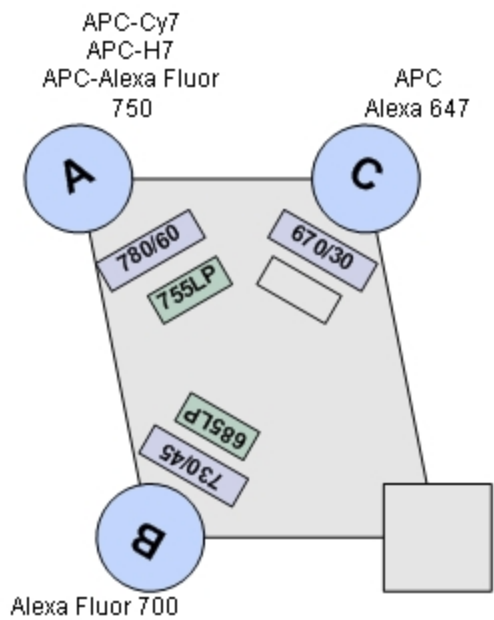

Comments: